

Sample Name :HIV-1 TAT (48-60)  
 Cat. No. : RP20423 Lot. No. :PE4731810  
 Time Processed : 21:06:17  
 Month-Day-Year Processed : 10/30/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

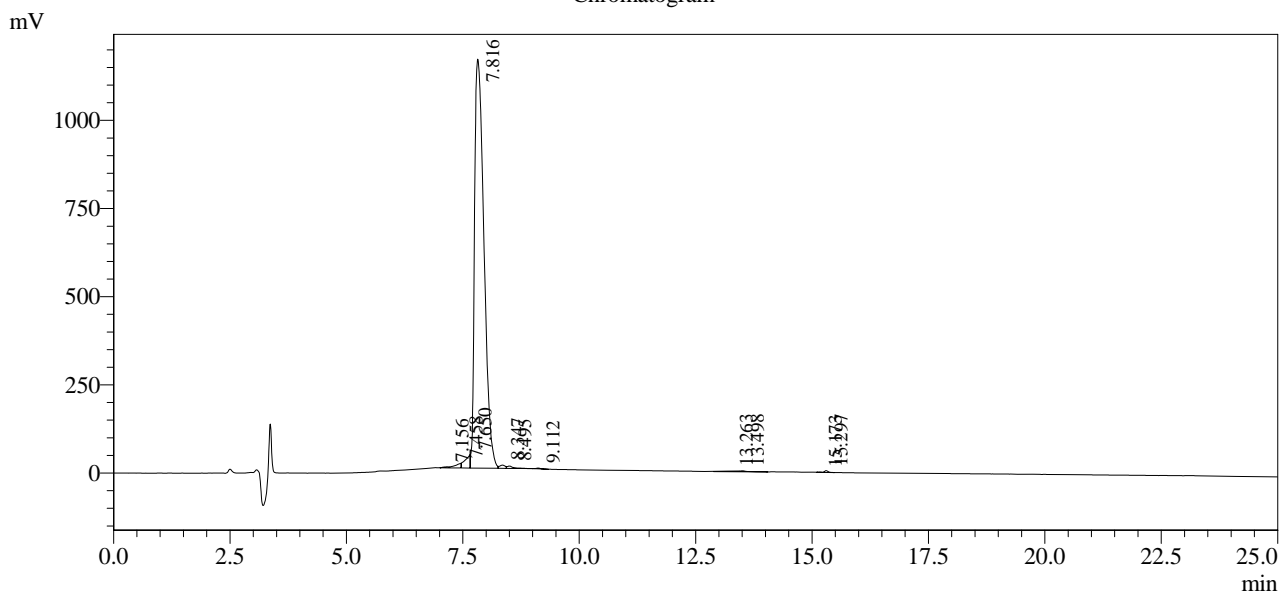

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.156	22385	2723	0.132
2	7.458	117710	13243	0.695
3	7.650	286519	36739	1.691
4	7.816	16259055	1159373	95.973
5	8.347	75661	9162	0.447
6	8.495	65427	6888	0.386
7	9.112	13398	2262	0.079
8	13.263	45478	2072	0.268
9	13.498	26912	2612	0.159
10	15.173	2832	561	0.017
11	15.297	25817	5031	0.152
Total		16941194	1240666	100.000