

Sample Name :Bombesin  
Cat. No. : RP11157  
Lot. No. :PE6151708

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

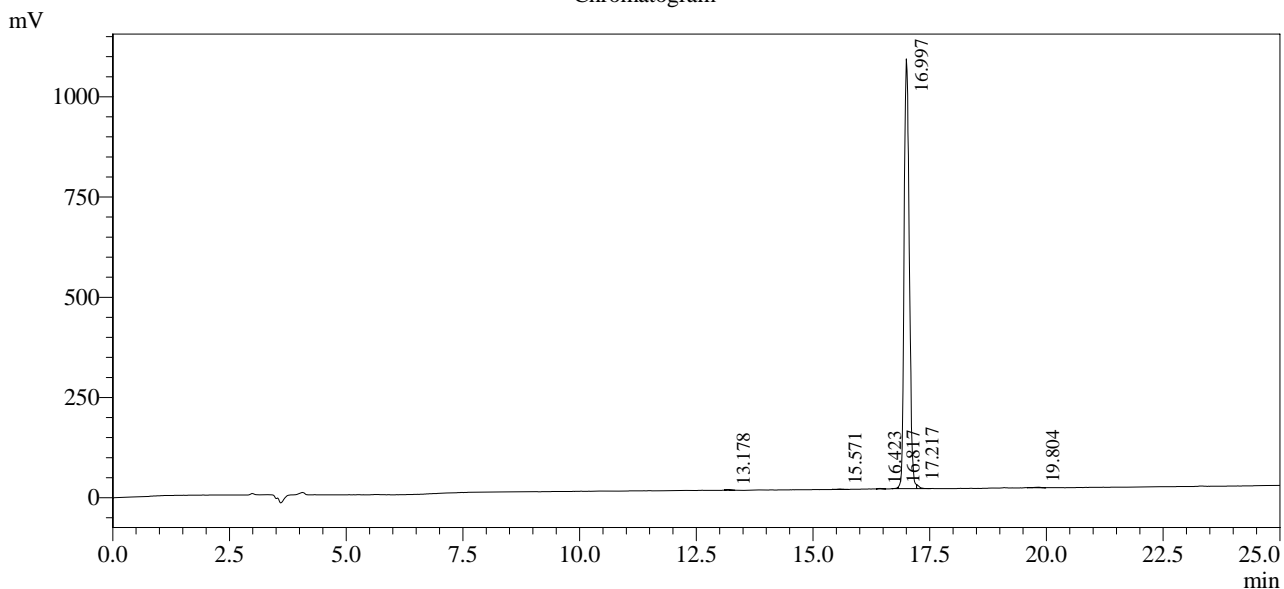

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.178	9672	1319	0.115
2	15.571	7458	1026	0.089
3	16.423	6394	1079	0.076
4	16.817	8398	3162	0.100
5	16.997	8308049	1071982	99.022
6	17.217	38151	10403	0.455
7	19.804	11953	1435	0.142
Total		8390076	1090406	100.000