


Mass Spectrum

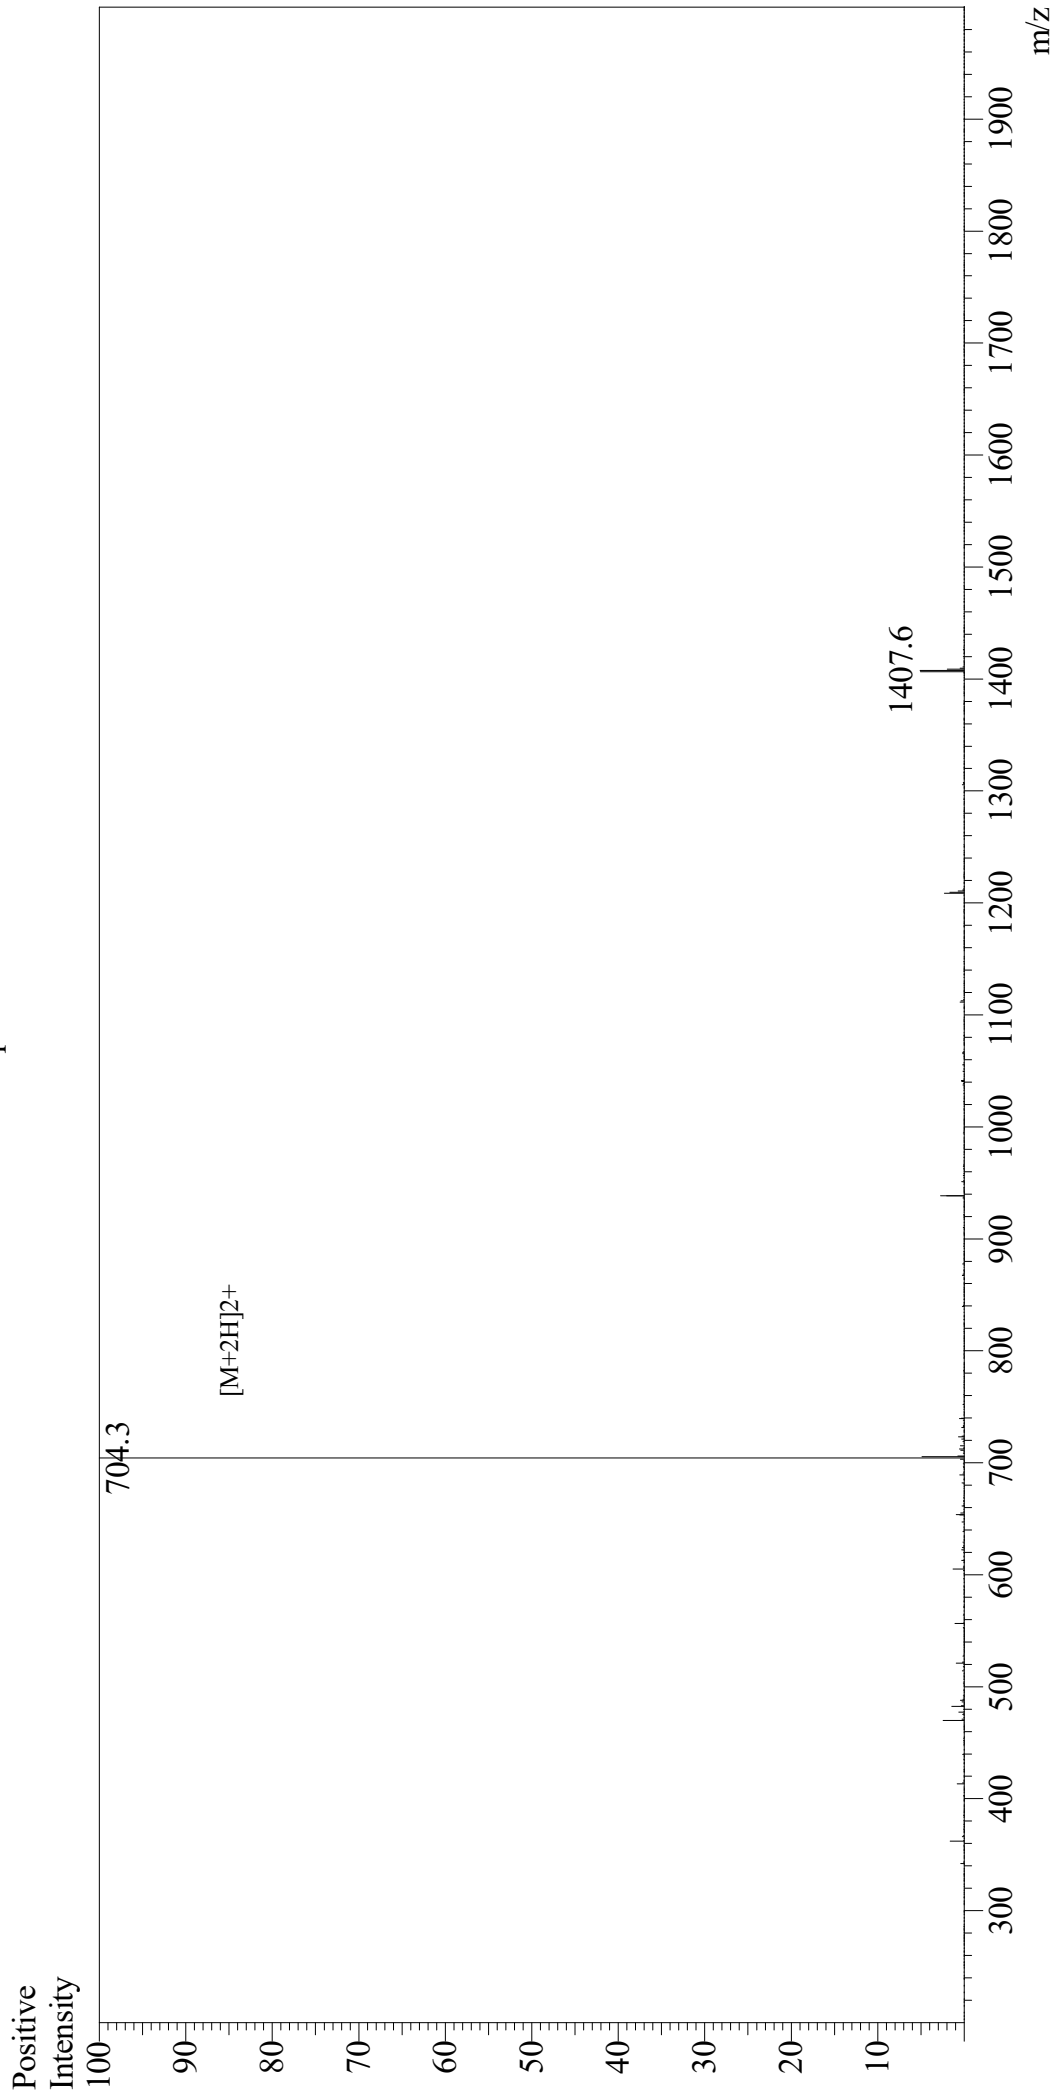

Sample Information

User : Gary
Month-Day Processed : 02/25/20
Time Processed : 07:09:13 PM
Injection Volume : 0.3
Sample Name : Hepatitis B Virus Core (128-140)
Cat No. : RP17313
Lot No. : E4777020B
Theoretical MW : 1406.63
Observed MW : 1406.6

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200