

Sample Name :Bradykinin
 Cat No. :RP11129
 Lot No. :PE0631812
 Time Processed : 13:14:33
 Month-Day-Year Processed : 12/15/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

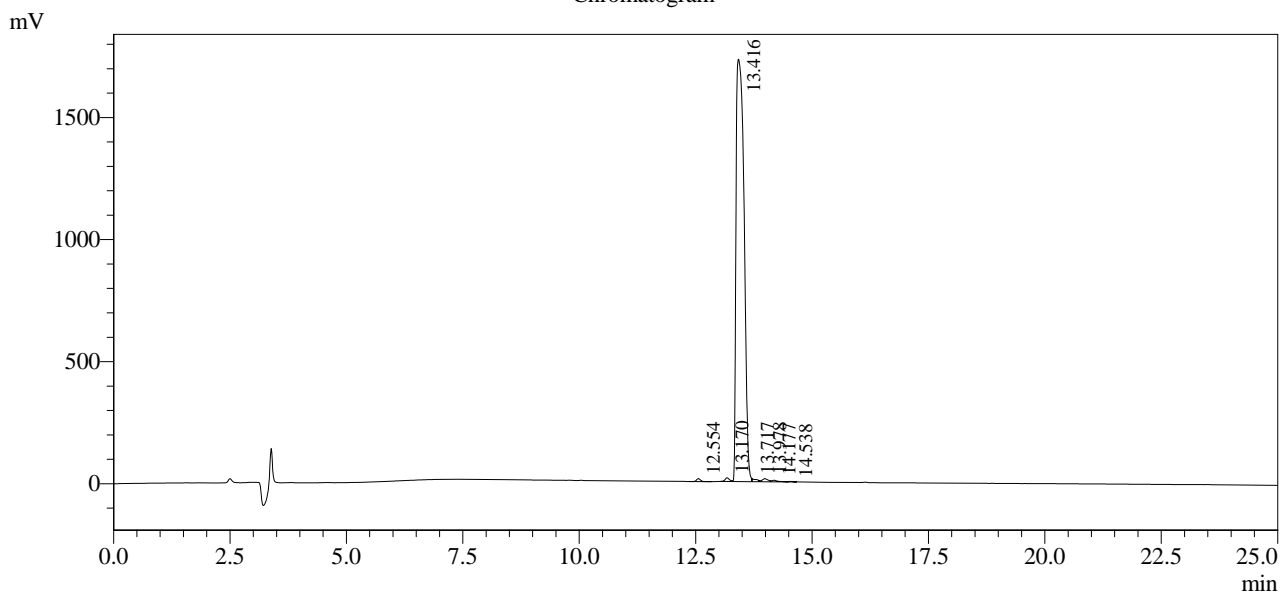

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.554	72874	12281	0.347
2	13.170	97216	15112	0.462
3	13.416	20599532	1729849	97.949
4	13.717	77569	11350	0.369
5	13.978	112919	13116	0.537
6	14.177	55447	6211	0.264
7	14.538	15408	2386	0.073
Total		21030966	1790305	100.000