

Sample Name : SV40 large T antigen NLS(RP20414)
 Cat. No. : RP20114
 Lot. No. : PE9271703

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

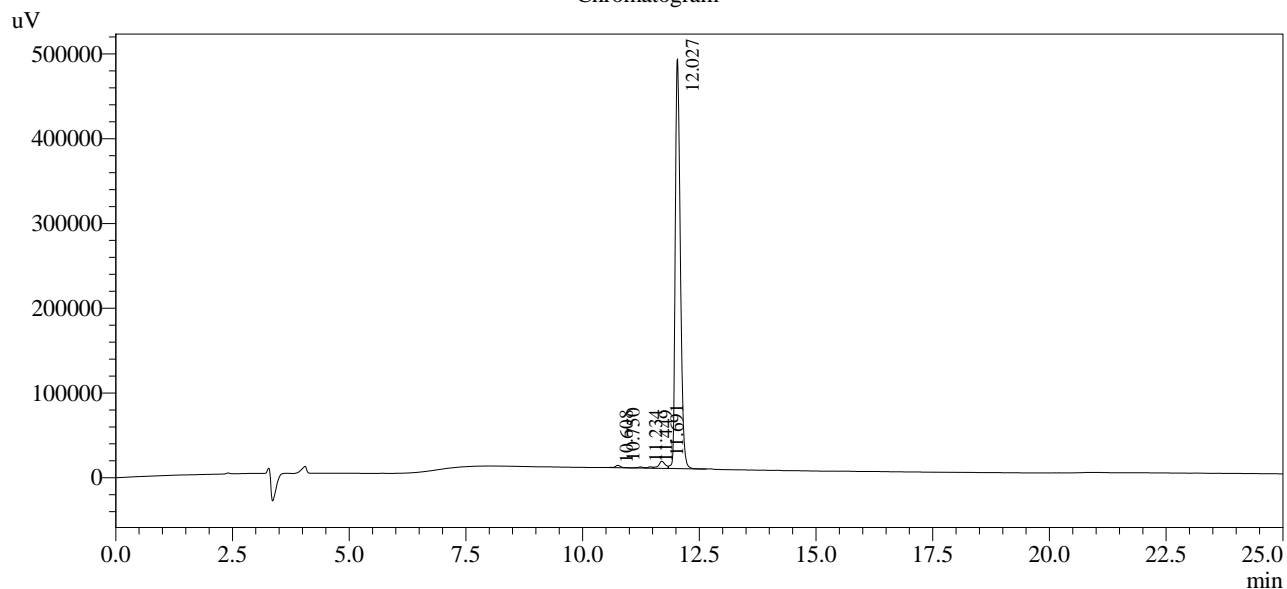

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.608	1186	249	0.031
2	10.750	21799	2776	0.575
3	11.234	11285	1344	0.298
4	11.449	11451	1617	0.302
5	11.691	82208	8392	2.168
6	12.027	3663180	483513	96.626
Total		3791110	497891	100.000