

Sample Name :N-Acetyl-Ser-Asp-Lys-Pro
 Cat No. :RP10555
 Lot No. : PE1101903
 Time Processed :10:51:50
 Month-Day-Year Processed :03/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	0	
5.00	Pumps	Pump B Conc.	0	
20.00	Pumps	Pump B Conc.	30	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	0	
40.00	Pumps	Pump B Conc.	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

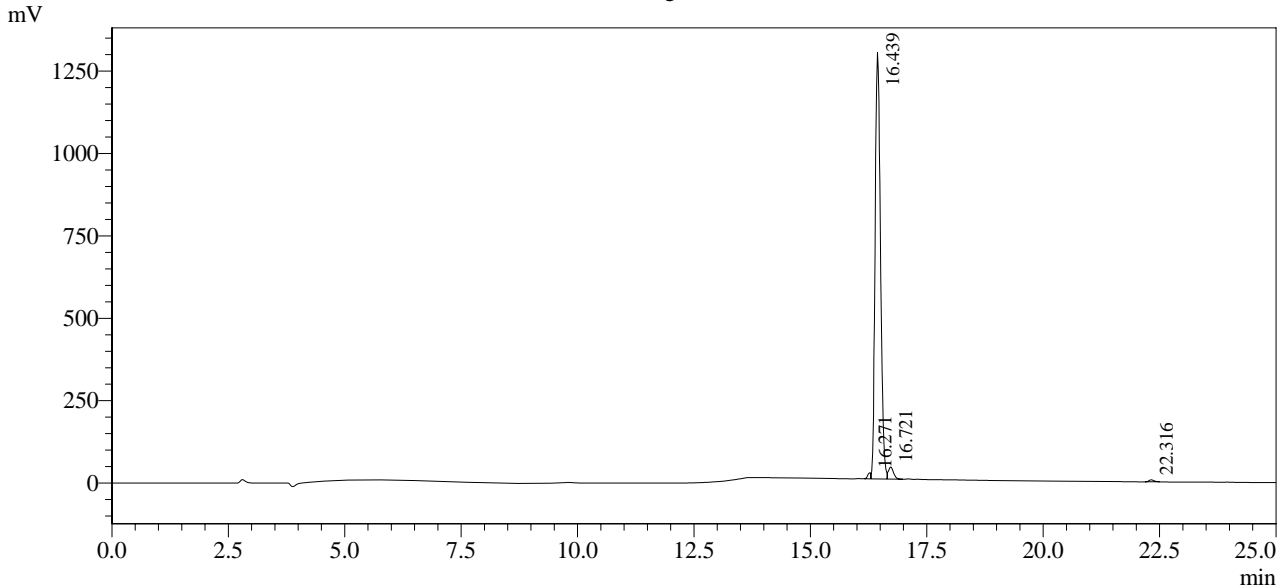

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.271	84065	18220	0.775
2	16.439	10444915	1293158	96.243
3	16.721	278796	36561	2.569
4	22.316	44859	6113	0.413
Total		10852634	1354053	100.000