

Sample Name : DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : PE7311612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

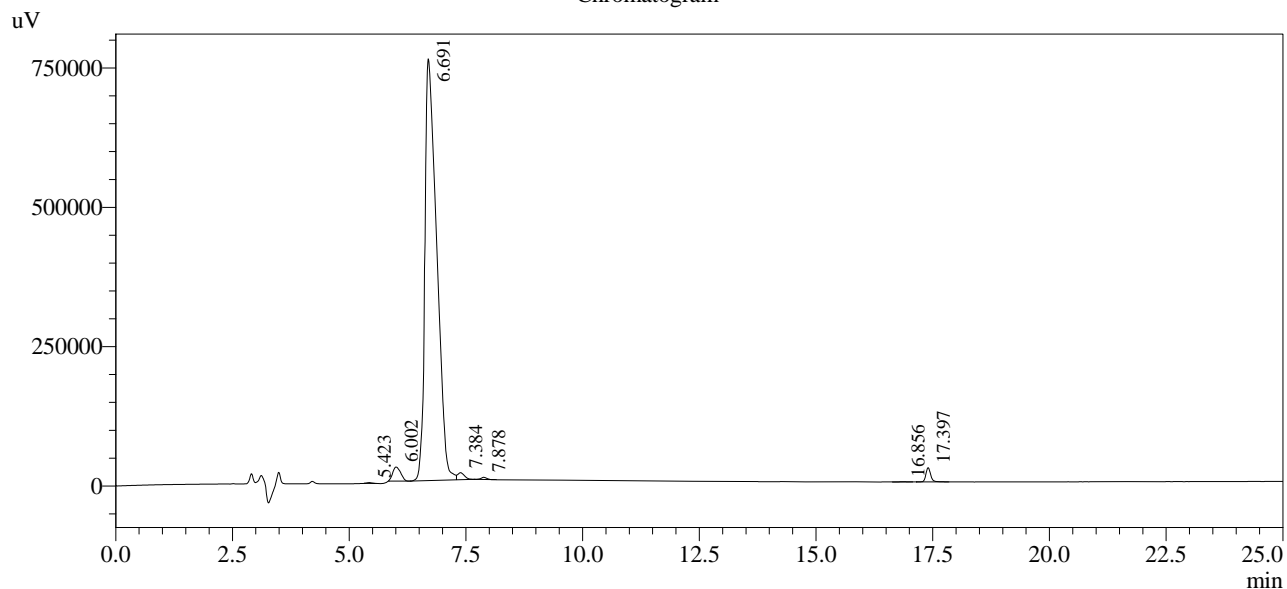

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.423	10324	1425	0.074
2	6.002	301473	25305	2.160
3	6.691	13295823	756915	95.253
4	7.384	130051	12768	0.932
5	7.878	33297	3999	0.239
6	16.856	4823	409	0.035
7	17.397	182616	25631	1.308
Total		13958407	826453	100.000