

Sample Name : Axl tide
 Cat. No. : RP20363
 Lot. No. : PE4371903
 Time Processed : 15:42:57
 Month-Day-Year Processed : 03/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

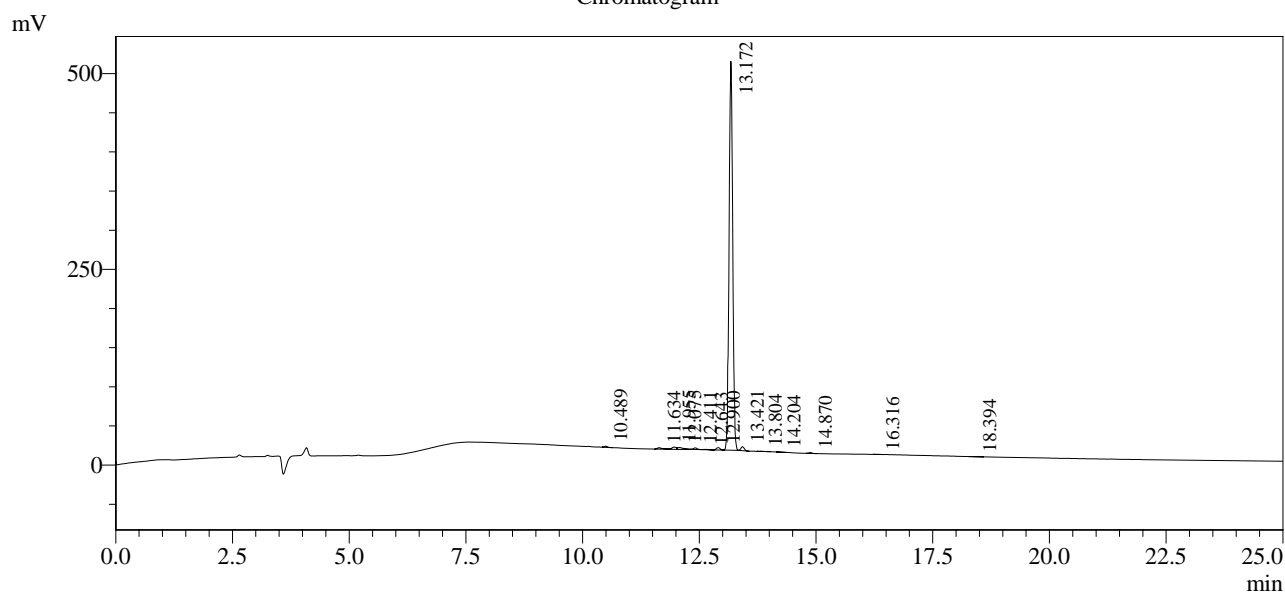

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.489	6630	1404	0.234
2	11.634	16300	1880	0.575
3	11.955	20282	2862	0.715
4	12.075	22934	2303	0.809
5	12.411	11238	2056	0.396
6	12.643	3270	445	0.115
7	12.900	17737	3107	0.626
8	13.172	2698727	496947	95.189
9	13.421	25535	5117	0.901
10	13.804	1648	220	0.058
11	14.204	2292	390	0.081
12	14.870	5326	1110	0.188
13	16.316	1223	201	0.043
14	18.394	1977	249	0.070
Total		2835119	518292	100.000