

Sample Name :SV40 large T antigen NLS
 Cat No.: RP20414
 Lot No.: E1211220G
 Time Processed :10:03:05
 Month-Day-Year Processed :07/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

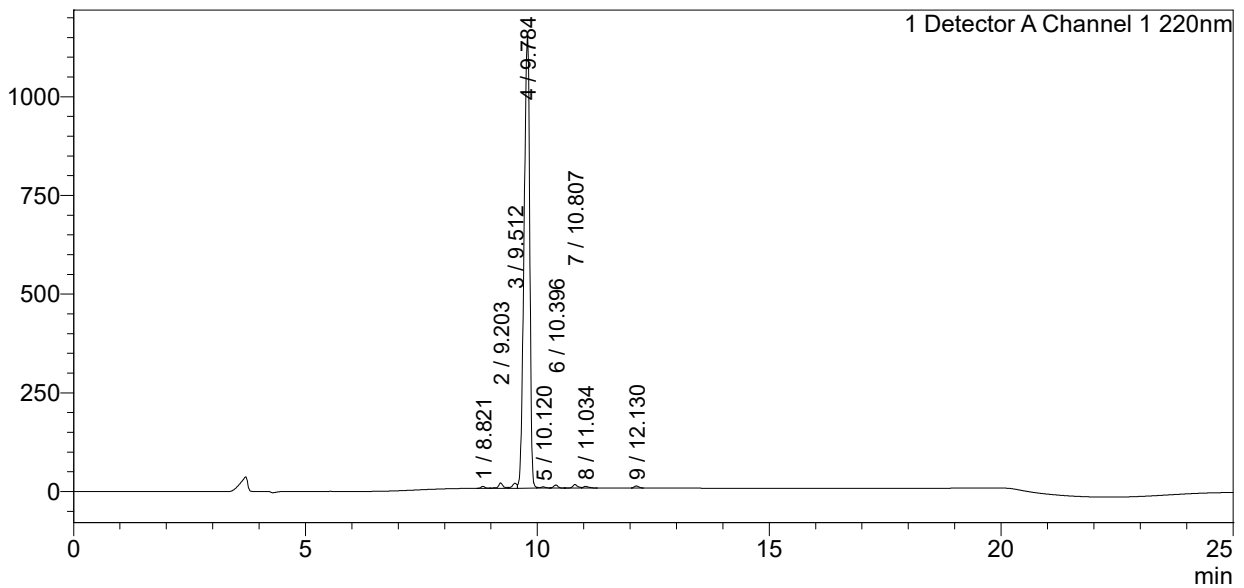

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.821	29206	4884	0.287
2	9.203	98589	13432	0.970
3	9.512	84110	12554	0.827
4	9.784	9736806	1145644	95.754
5	10.120	30020	3357	0.295
6	10.396	52671	8012	0.518
7	10.807	68280	9044	0.671
8	11.034	35033	4458	0.345
9	12.130	33805	5134	0.332
Total		10168520	1206519	100.000