

Sample Name :Angiotensin II, human

Cat. No. : RP11257 Lot. No. : PE7381808

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

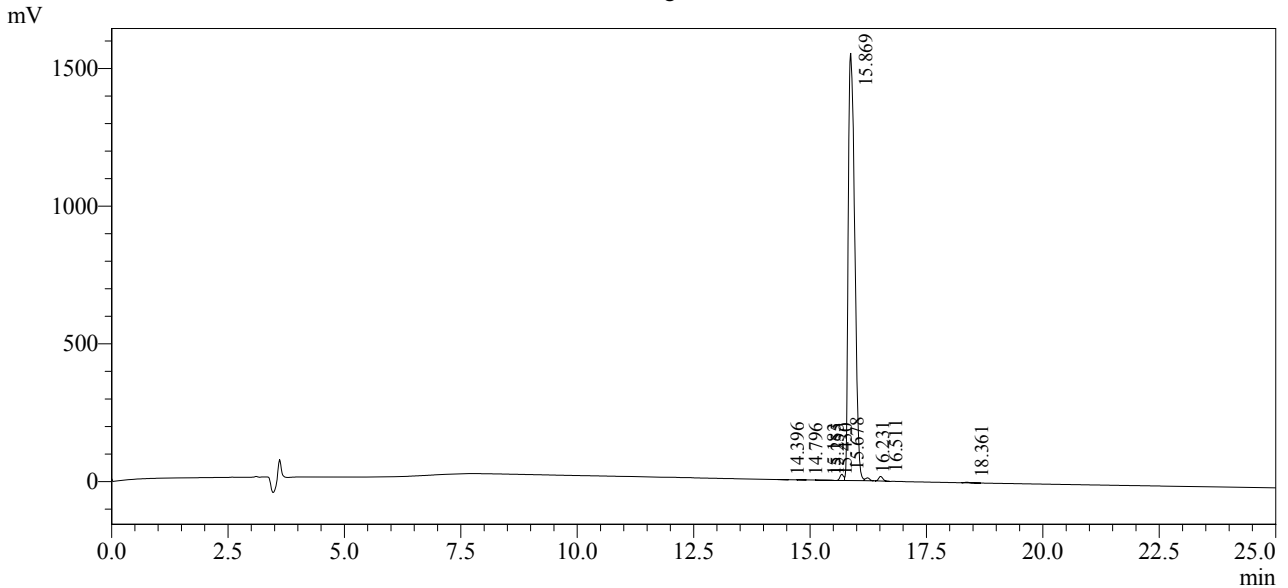

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.396	6071	1130	0.039
2	14.796	2822	552	0.018
3	15.183	1887	476	0.012
4	15.255	4530	720	0.029
5	15.430	8440	1206	0.055
6	15.678	126918	22869	0.823
7	15.869	15080065	1551220	97.844
8	16.231	62589	10395	0.406
9	16.511	104588	16830	0.679
10	18.361	14440	2392	0.094
Total		15412349	1607789	100.000