


Mass Spectrum

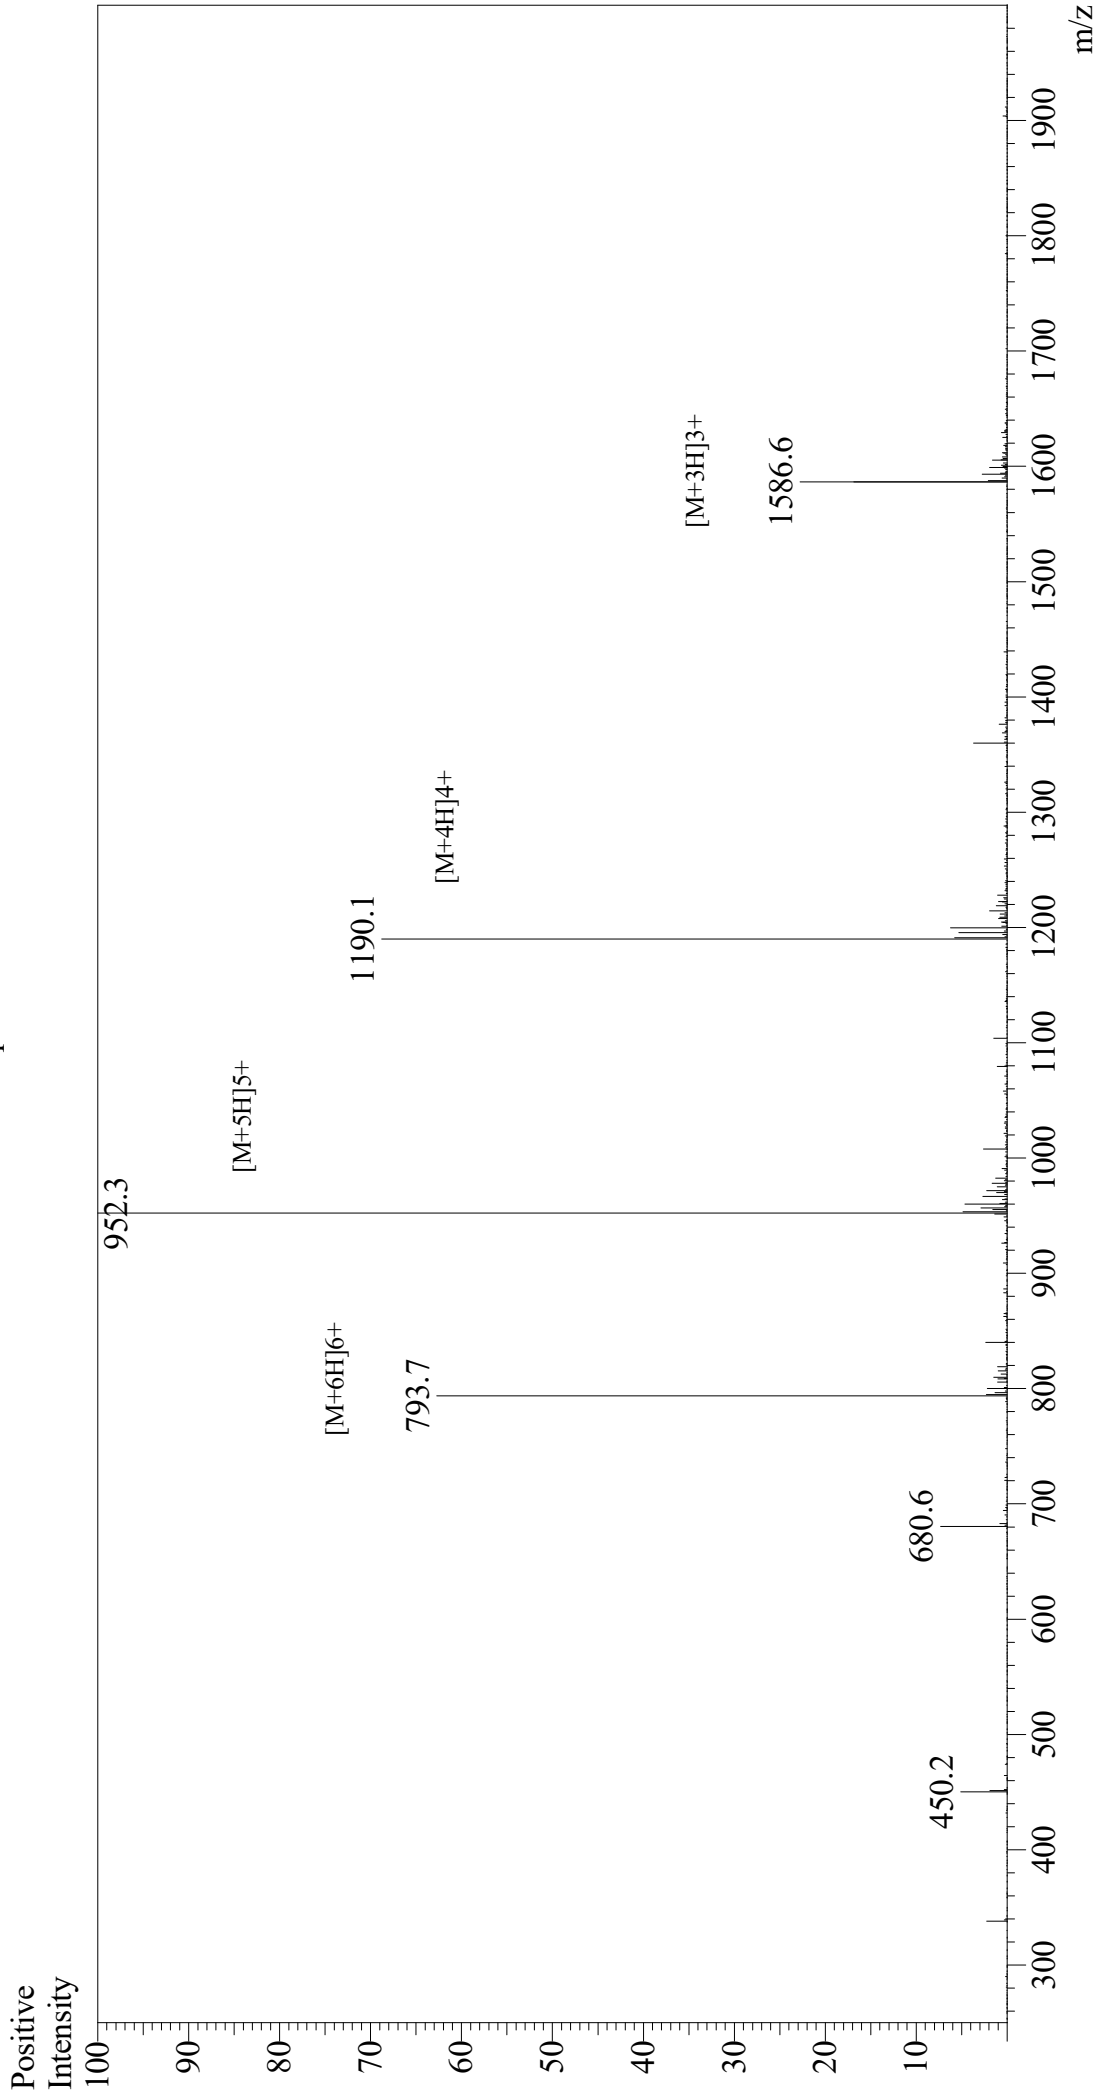

Sample Information
Month-Day Processed : 03/10/21
Time Processed : 10:05:45 AM
Injection Volume : 0.6
Sample Name : Corticotropin Releasing Factor, human, rat
Cat No. : RP10982
Lot No. : E8086321C
Theoretical MW : 4757.45
Observed MW : 4756.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH