

Sample Name :Dermorphin
 Cat No. :RP10427
 Lot No. :E4808519I
 Time Processed :16:01:09
 Month-Day-Year Processed :09/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

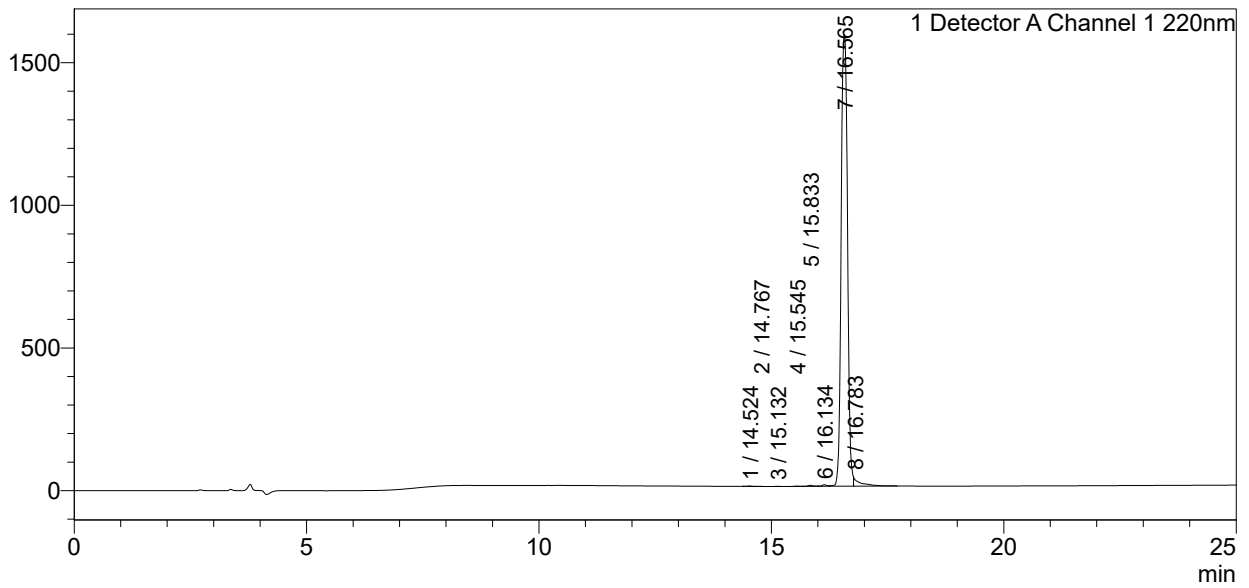

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.524	10115	1505	0.066
2	14.767	1408	186	0.009
3	15.132	2762	404	0.018
4	15.545	4355	743	0.028
5	15.833	29946	3497	0.196
6	16.134	39429	5172	0.258
7	16.565	14921959	1578296	97.504
8	16.783	293906	27477	1.920
Total		15303880	1617281	100.000