

Sample Name :Bid BH3 Peptide
 Cat No. :RP20440
 Lot No. :E4962719I
 Time Processed :8:26:18 AM
 Month-Day-Year Processed :10/06/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

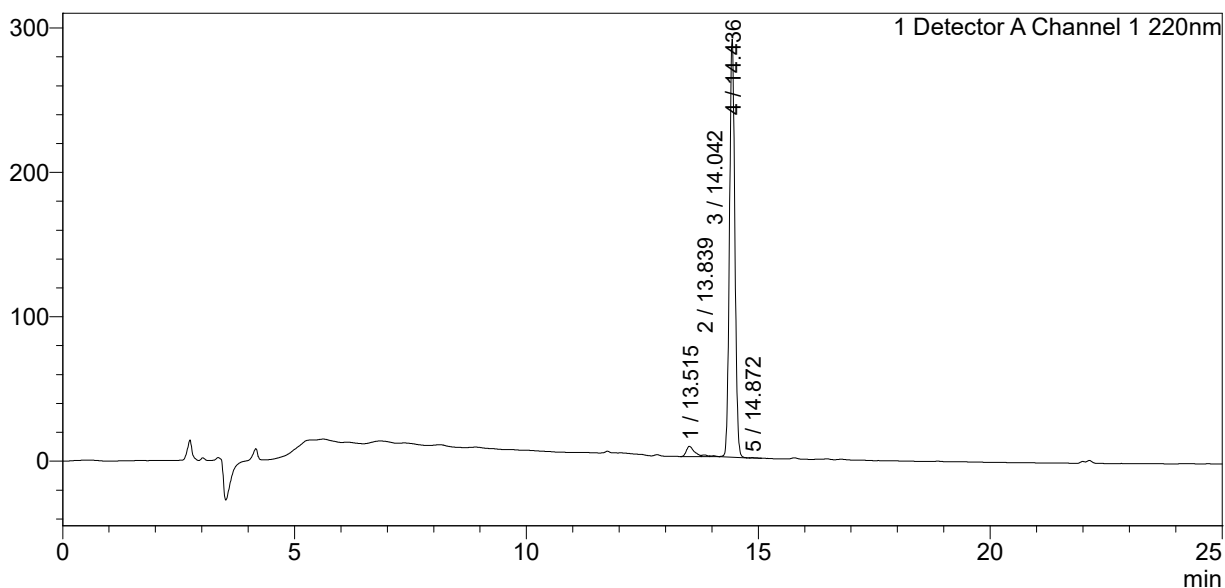

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.515	82824	7113	3.408
2	13.839	8814	1145	0.363
3	14.042	3965	549	0.163
4	14.436	2333388	289565	96.019
5	14.872	1141	131	0.047
Total		2430132	298502	100.000