

Sample Name :Chemerin-9 (149-157)  
 Cat No. :RP20248  
 Lot No. :E7836121E  
 Time Processed :21:07:30  
 Month-Day-Year Processed :05/08/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

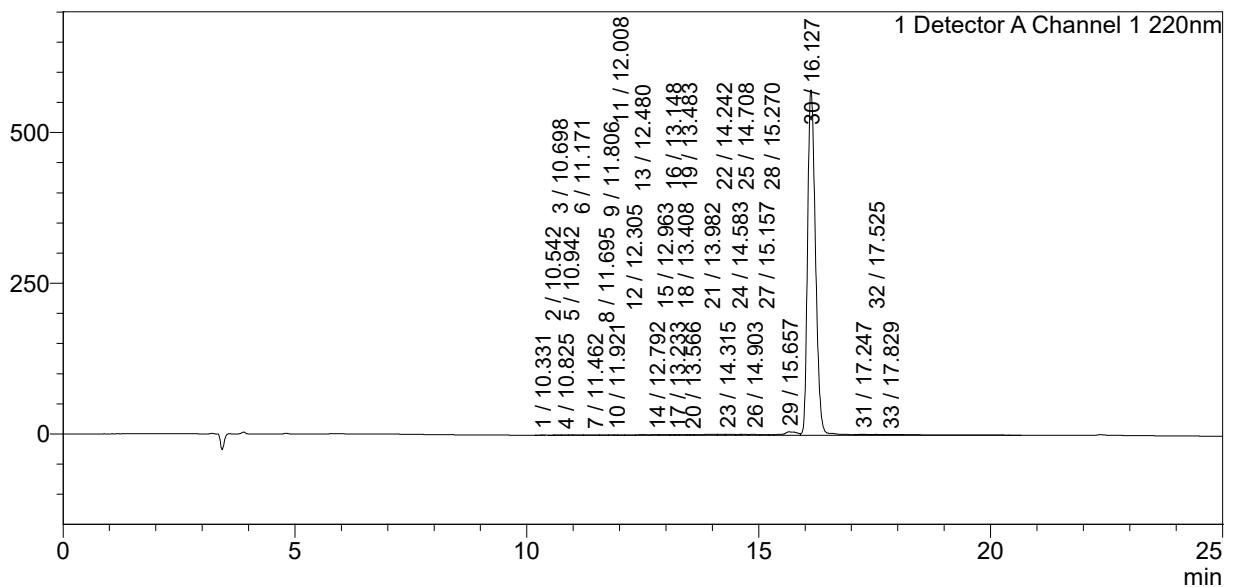

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.331	1289	162	0.018
2	10.542	1033	135	0.014
3	10.698	1652	212	0.023
4	10.825	2015	222	0.028
5	10.942	1368	256	0.019
6	11.171	4361	391	0.060
7	11.462	10022	562	0.138
8	11.695	5913	551	0.081
9	11.806	3682	512	0.051
10	11.921	2189	497	0.030
11	12.008	4539	522	0.062
12	12.305	7611	582	0.105
13	12.480	13633	962	0.187
14	12.792	9495	792	0.130

Peak#	Ret. Time	Area	Height	Area%
15	12.963	10766	790	0.148
16	13.148	4706	804	0.065
17	13.233	4264	785	0.059
18	13.408	8146	849	0.112
19	13.483	3851	862	0.053
20	13.566	4331	876	0.060
21	13.982	36743	1597	0.505
22	14.242	13051	1330	0.179
23	14.315	17795	1349	0.245
24	14.583	7865	1219	0.108
25	14.708	12461	1291	0.171
26	14.903	17363	1260	0.239
27	15.157	13727	1174	0.189
28	15.270	6994	1187	0.096
29	15.657	112567	5541	1.547
30	16.127	6925526	572587	95.180
31	17.247	3545	375	0.049
32	17.525	2574	314	0.035
33	17.829	1167	127	0.016
Total		7276247	600674	100.000