

Sample Name : Arg-Gly-Asp-Ser
 Cat. No. : RP10861
 Lot. No. : E5726619K
 Time Processed :6:53:26
 Month-Day-Year Processed :11/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

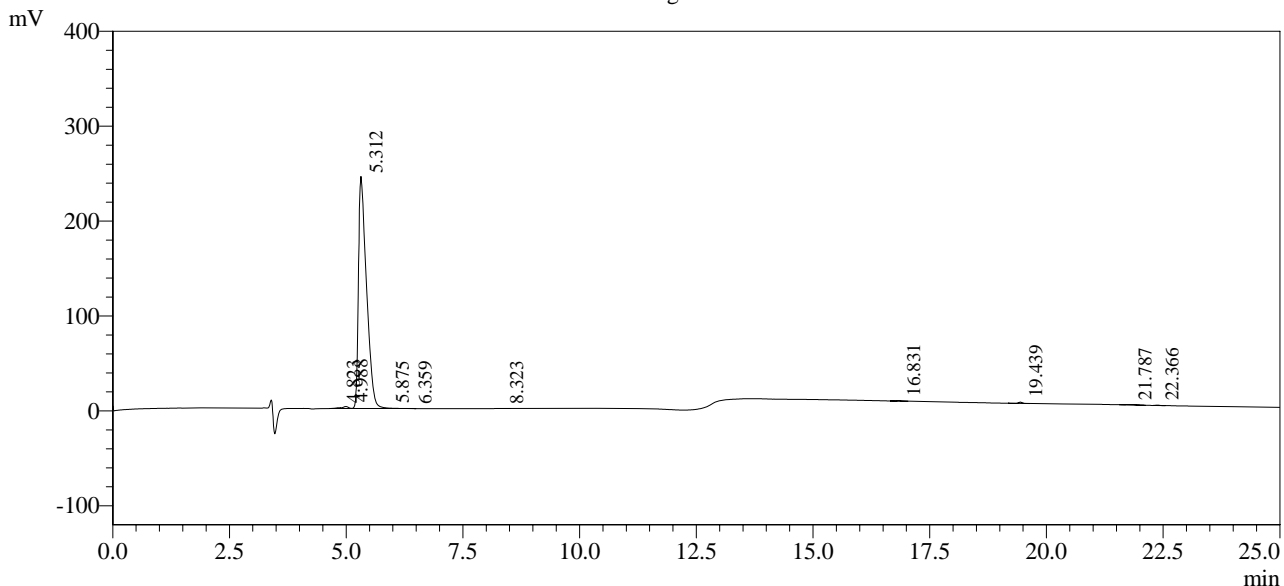

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.823	6047	832	0.203
2	4.988	18179	2118	0.610
3	5.312	2933893	244663	98.381
4	5.875	4586	551	0.154
5	6.359	151	31	0.005
6	8.323	1857	222	0.062
7	16.831	2886	508	0.097
8	19.439	7870	1416	0.264
9	21.787	4556	300	0.153
10	22.366	2164	397	0.073
Total		2982188	251038	100.000