

Sample Name : PAR2 AP  
 Cat No. : RP19975  
 Lot No. : E8098821C  
 Time Processed: 15:26:11  
 Year-Month-Day: 2021/3/10

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min

<<Detector A>>  
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010015

<Chromatogram>

mV

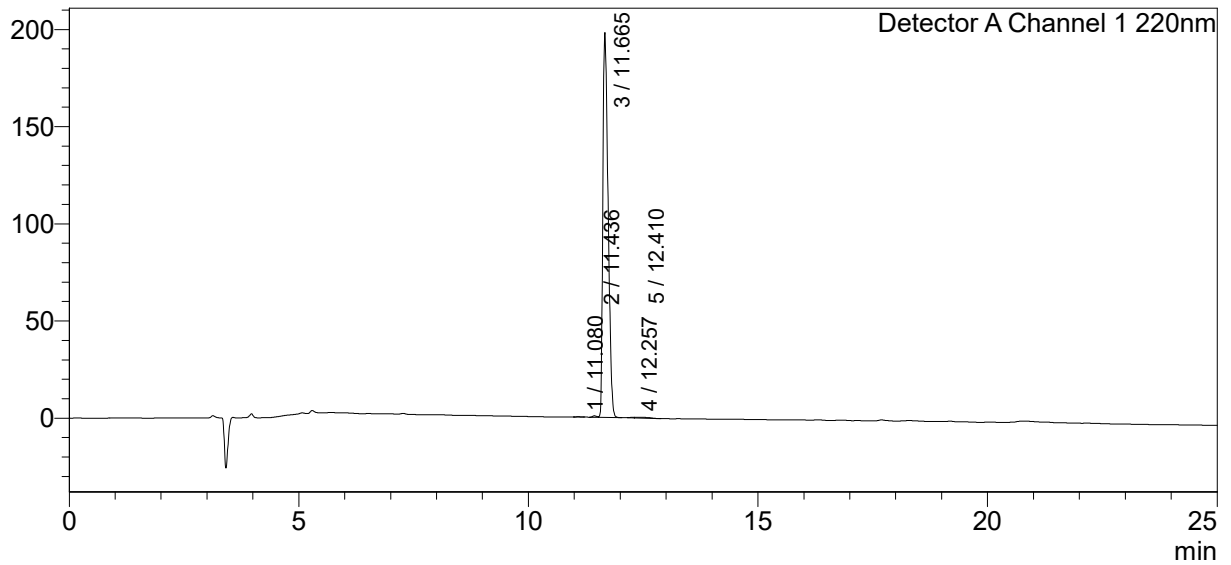

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.080	1432	221	0.090
2	11.436	4895	733	0.307
3	11.665	1576400	198047	98.967
4	12.257	1634	257	0.103
5	12.410	8499	400	0.534
Total		1592859	199659	100.000