

Sample Name :Angiotensin II, human
 Cat No. :RP11257
 Lot No. :E9410521D
 Time Processed :2:47:33 AM
 Month-Day-Year Processed :04/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

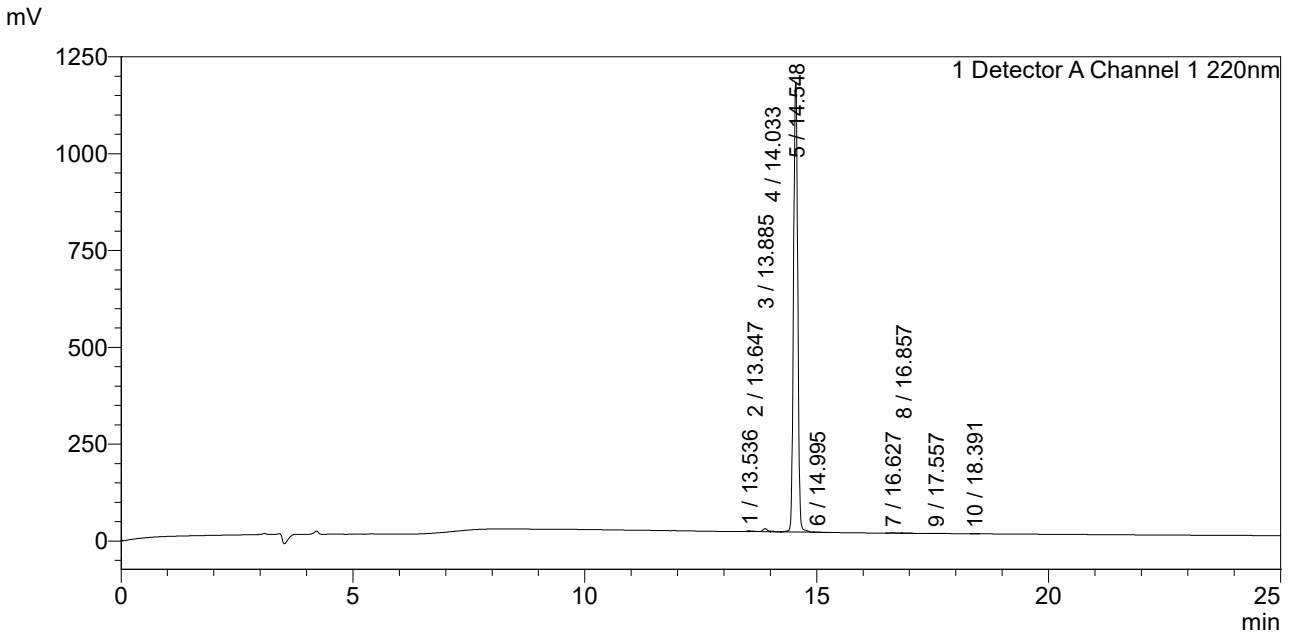

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.536	13950	2511	0.189
2	13.647	5454	1260	0.074
3	13.885	52751	7930	0.713
4	14.033	7042	1468	0.095
5	14.548	7299468	1160506	98.651
6	14.995	5861	748	0.079
7	16.627	8459	1181	0.114
8	16.857	1429	74	0.019
9	17.557	3327	275	0.045
10	18.391	1552	263	0.021
Total		7399292	1176216	100.000