

Sample Name :Neuromedin B

Cat No. :RP10507

Lot No. :PE5321805

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

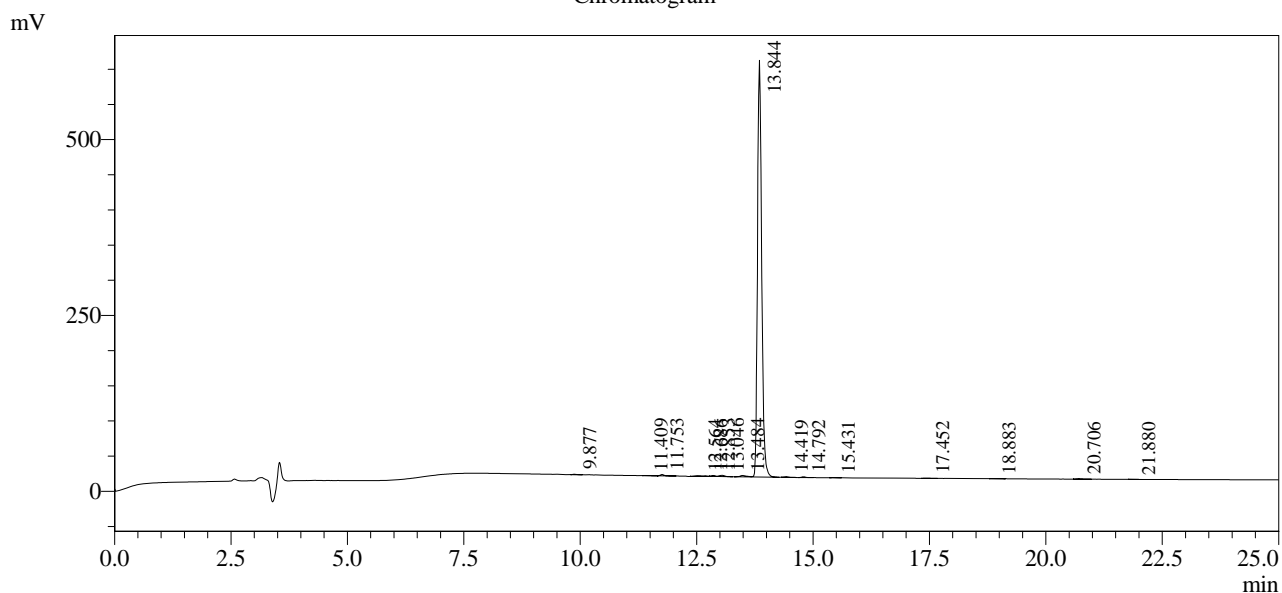

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.877	3581	687	0.094
2	11.409	1941	232	0.051
3	11.753	11788	1967	0.310
4	12.564	4324	498	0.114
5	12.686	2005	447	0.053
6	12.853	7012	1218	0.184
7	13.046	14340	1738	0.377
8	13.484	19200	1917	0.504
9	13.844	3721763	592293	97.754
10	14.419	4186	718	0.110
11	14.792	6241	1066	0.164
12	15.431	1881	309	0.049
13	17.452	2398	311	0.063
14	18.883	1949	305	0.051
15	20.706	3318	405	0.087
16	21.880	1364	180	0.036
Total		3807290	604289	100.000