

Sample Name :VIP, human, ovine, porcine, rat
 Cat No.: RP10085
 Lot No.: E3656520A
 Time Processed :22:09:04
 Month-Day-Year Processed :01/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

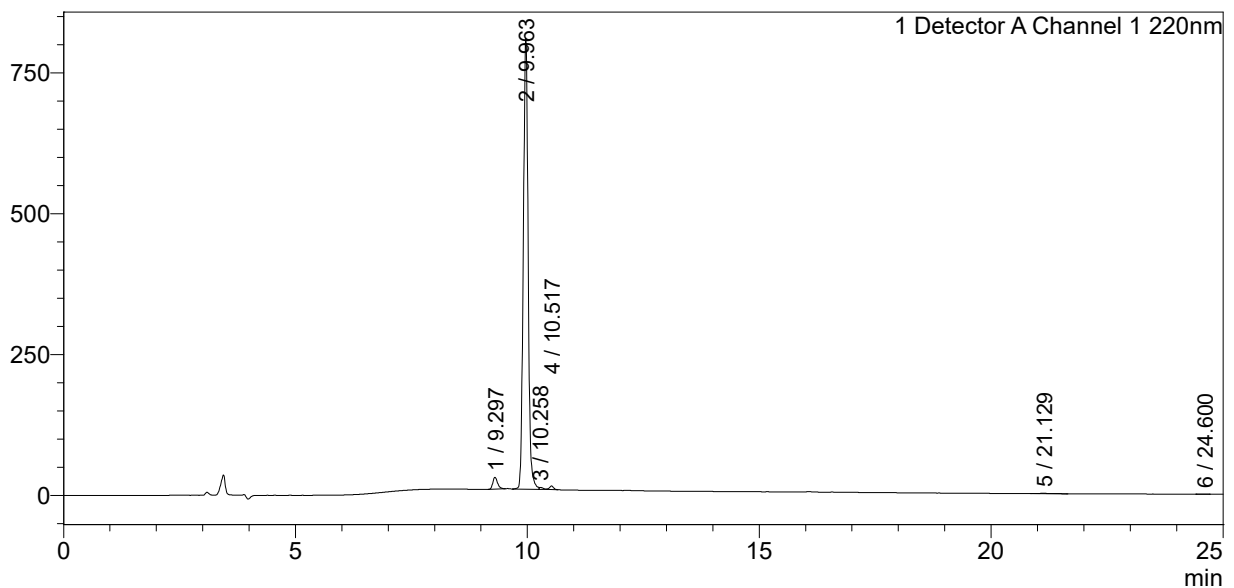

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.297	148386	20932	2.485
2	9.963	5751689	801337	96.337
3	10.258	21535	3490	0.361
4	10.517	36609	6311	0.613
5	21.129	10655	556	0.178
6	24.600	1491	150	0.025
Total		5970366	832776	100.000