

Sample Name :Proctolin  
 Cat No. :RP10475  
 Lot No. :E4801119I  
 Time Processed :1:40:35 PM  
 Month-Day-Year Processed :09/23/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

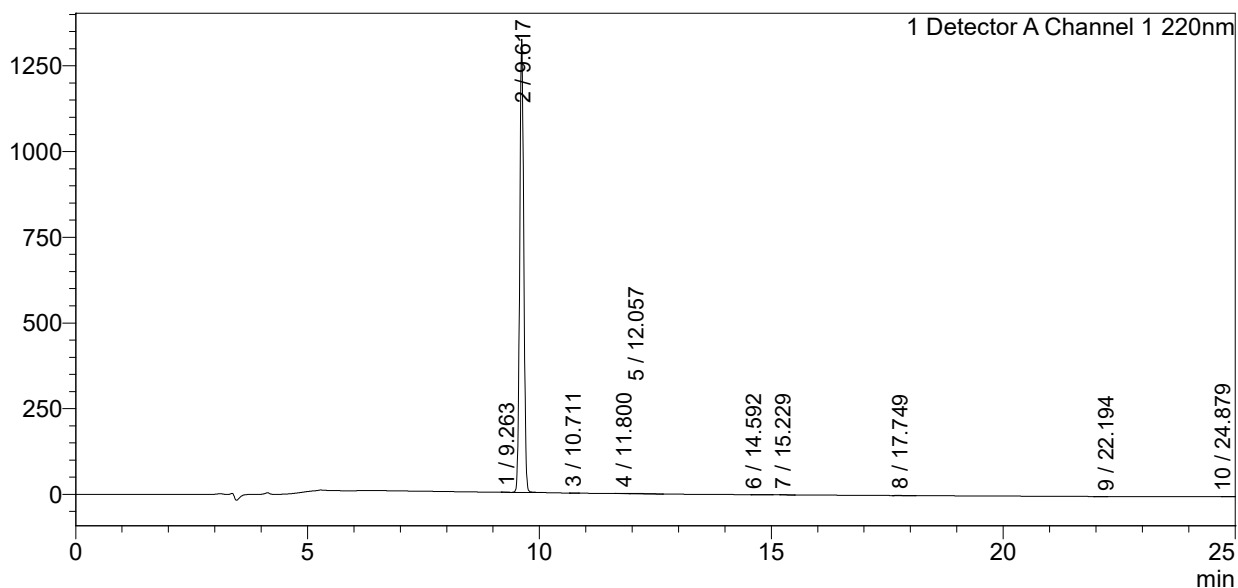

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.263	4206	736	0.052
2	9.617	8050625	1322541	99.437
3	10.711	1021	201	0.013
4	11.800	7609	489	0.094
5	12.057	25416	1077	0.314
6	14.592	1075	43	0.013
7	15.229	1006	64	0.012
8	17.749	2319	207	0.029
9	22.194	1198	102	0.015
10	24.879	1734	207	0.021
Total		8096210	1325667	100.000