

Sample Name : Exendin-4
 Cat No. : RP10874
 Lot No. : E7242421A
 Time Processed : 3:40:25 PM
 Month-Day-Year Processed : 01/16/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Module	Command	Value
0.01	Pumps	B.Conc	15
25.00	Pumps	B.Conc	75
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	15
40.00	Pumps	B.Conc	15
60.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

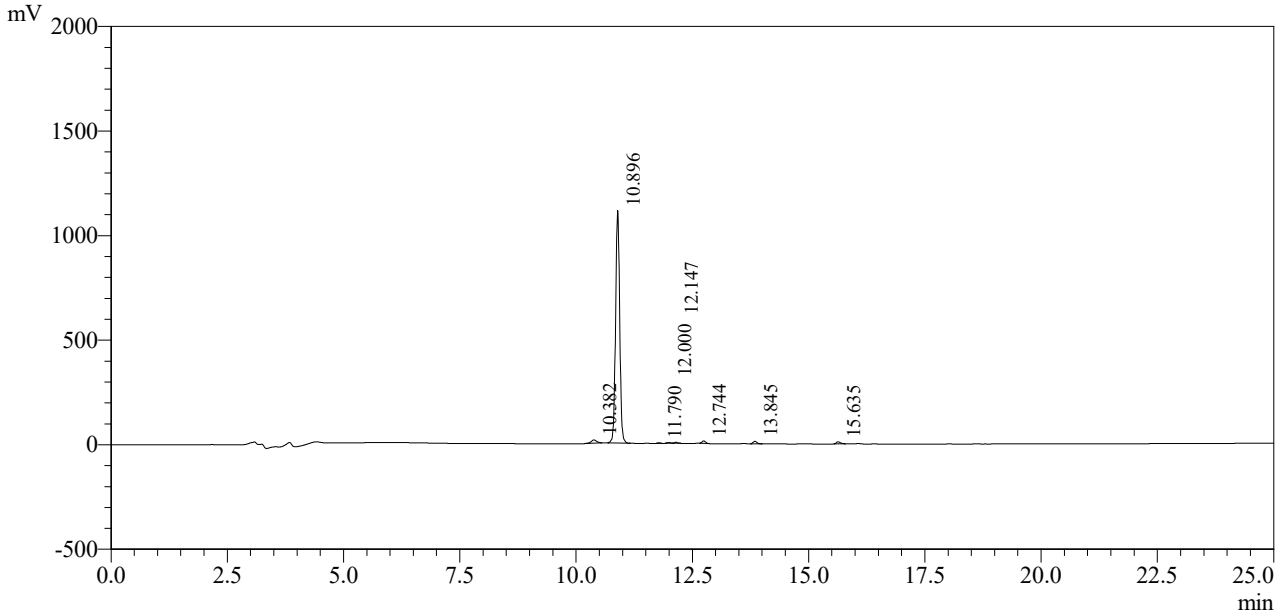

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.382	124925	14978	1.722
2	10.896	6899135	1111680	95.120
3	11.790	9064	2315	0.125
4	12.000	17853	3832	0.246
5	12.147	19944	4561	0.275
6	12.744	62084	11693	0.856
7	13.845	63809	11366	0.880
8	15.635	56300	9570	0.776
Total		7253115	1169996	100.000