

Sample Name :SV40 large T antigen NLS
 Cat. No. : RP20414
 Lot. No. : PE4301902
 Time Processed : 9:37:04
 Month-Day-Year Processed : 02/15/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

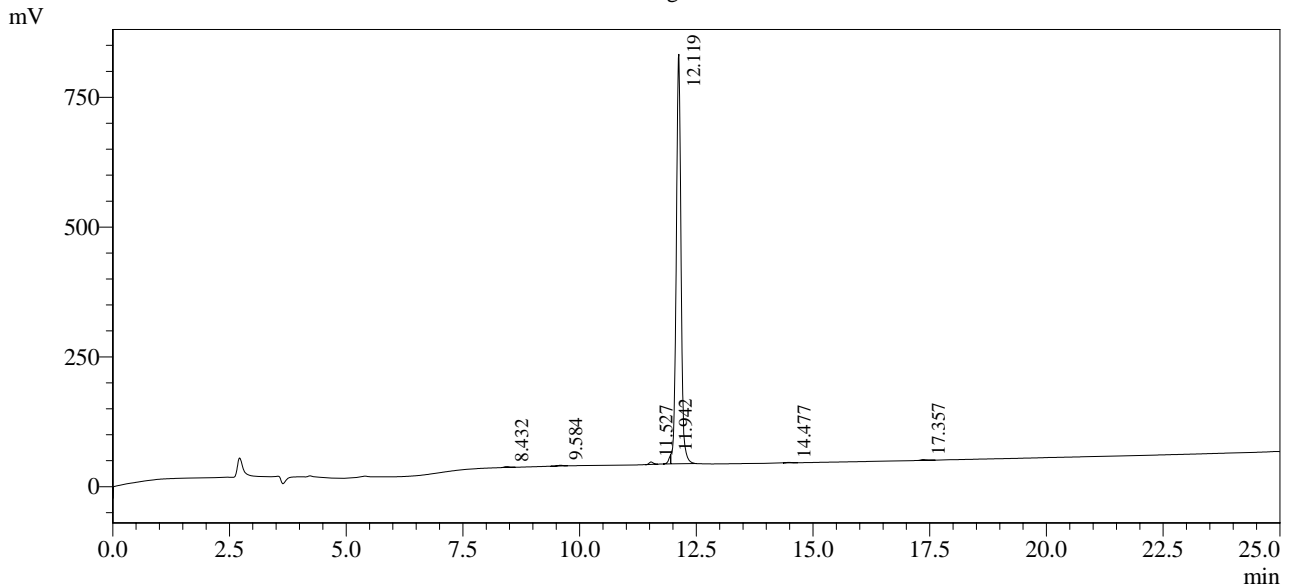

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.432	11411	1550	0.201
2	9.584	10050	1362	0.177
3	11.527	29308	4808	0.515
4	11.942	52681	16196	0.926
5	12.119	5567793	788755	97.901
6	14.477	6509	906	0.114
7	17.357	9395	1460	0.165
Total		5687149	815036	100.000