

Sample Name :Kemptide (Phospho-Ser5)  
 Cat No.: RP20111  
 Lot No.:E4830519I  
 Time Processed :12:28:04  
 Month-Day-Year Processed :09/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

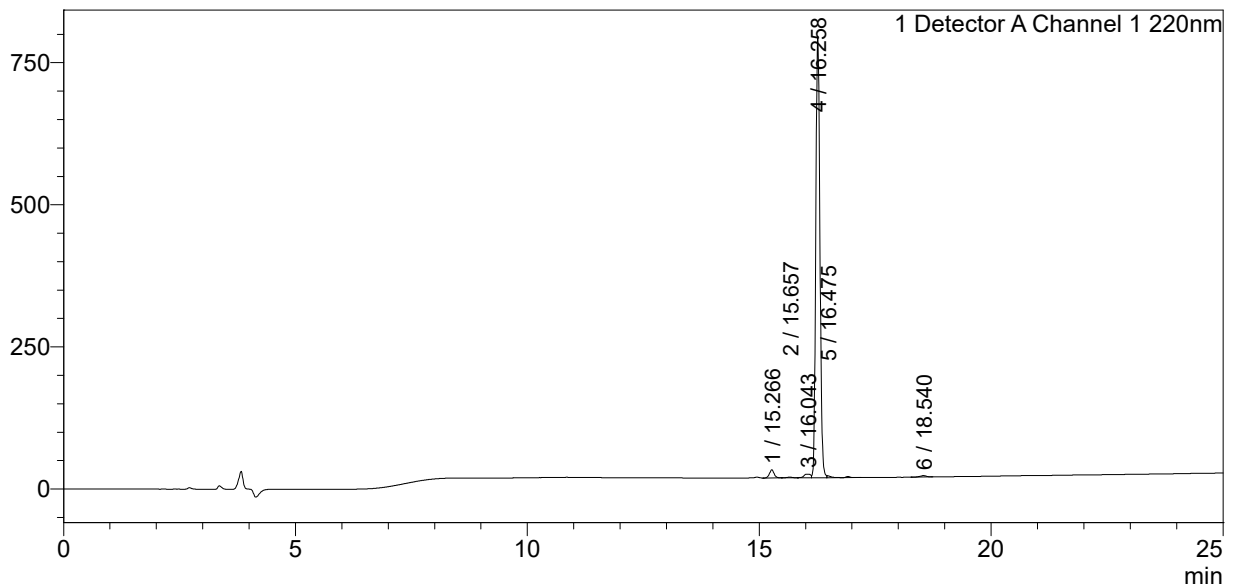

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.266	100569	14198	1.964
2	15.657	12565	1377	0.245
3	16.043	65612	6480	1.281
4	16.258	4879945	762947	95.307
5	16.475	36202	3610	0.707
6	18.540	25343	2560	0.495
Total		5120237	791172	100.000