

Sample Name :Melittin
 Cat No :RP10290
 Lot No :E8678321F
 Time Processed :1:25:45
 Month-Day-Year Processed :06/23/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------|-------|
| 0.01 | Pumps | B.Conc | 5 |
| 25.00 | Pumps | B.Conc | 65 |
| 25.01 | Pumps | B.Conc | 95 |
| 27.00 | Pumps | B.Conc | 95 |
| 27.01 | Pumps | B.Conc | 5 |
| 35.00 | Pumps | B.Conc | 5 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

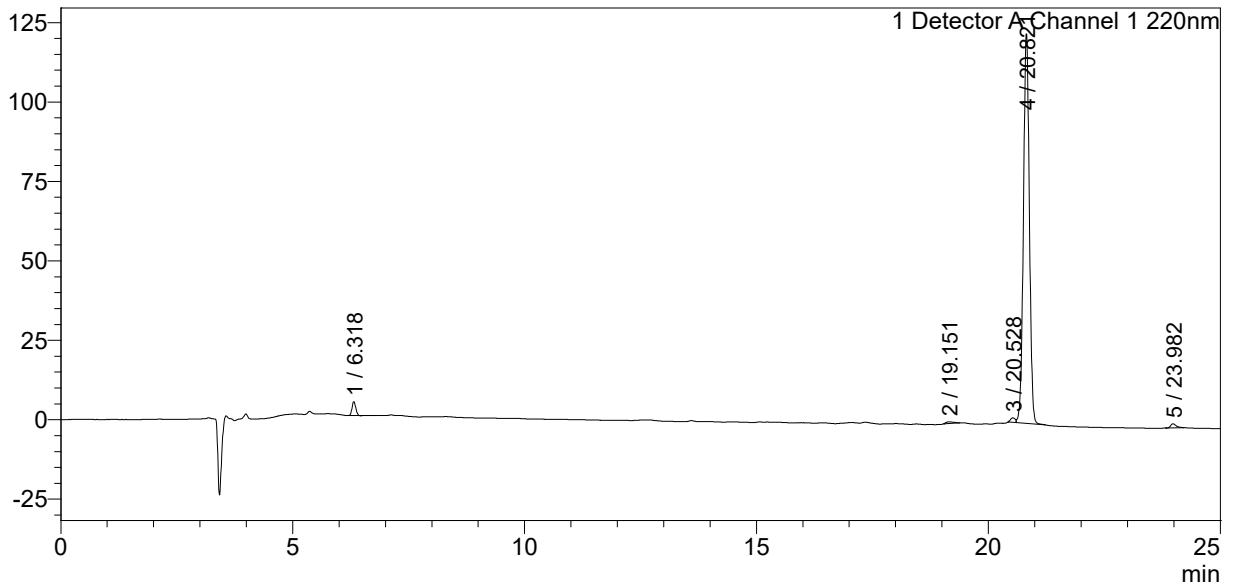

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 6.318 | 24412 | 4394 | 2.140 |
| 2 | 19.151 | 5480 | 512 | 0.480 |
| 3 | 20.528 | 9990 | 1401 | 0.876 |
| 4 | 20.821 | 1090444 | 122589 | 95.602 |
| 5 | 23.982 | 10281 | 1283 | 0.901 |
| Total | | 1140607 | 130179 | 100.000 |