

Sample Name: Kemptide
 Cat No. : RP10287
 Lot No. : E1559220A
 Time Processed: 1:25:29 PM
 Month-Day-Year Processed :01/19/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	15
25.00	Pumps	Solvent B Conc.	75
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	15
40.00	Pumps	Solvent B Conc.	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

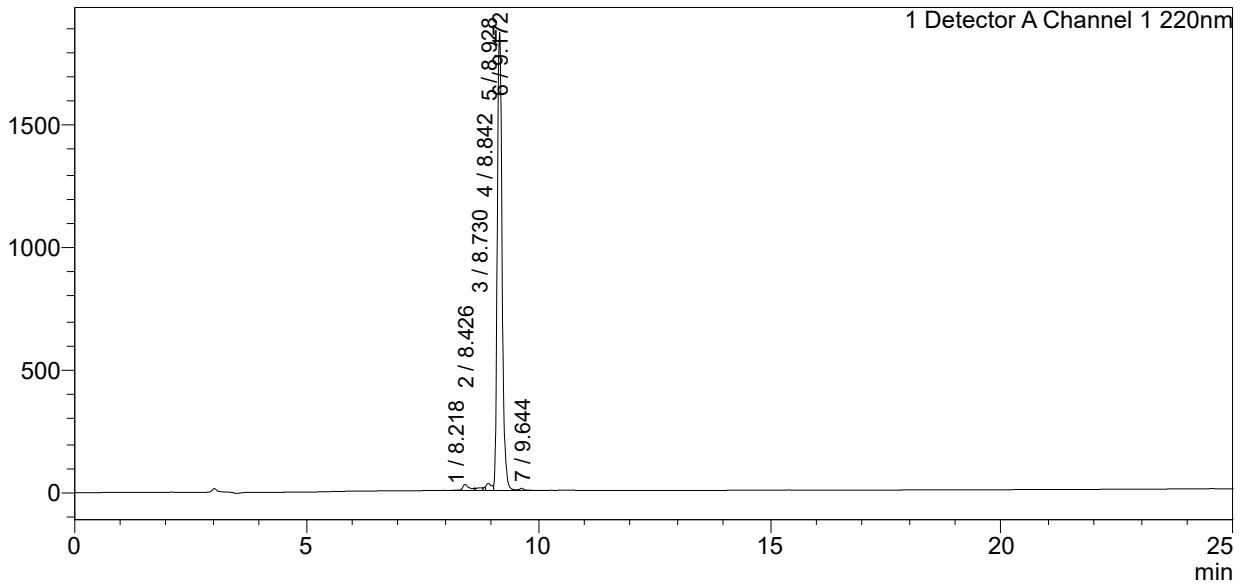

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.218	3426	654	0.024
2	8.426	224720	24029	1.578
3	8.730	90837	10584	0.638
4	8.842	36599	11272	0.257
5	8.928	220762	28357	1.550
6	9.172	13606556	1871788	95.525
7	9.644	61007	8529	0.428
Total		14243908	1955213	100.000