

Sample Name :Palmitoyl Tetrapeptide-3
 Cat No. :RP20100
 Lot No. :E4830019I
 Time Processed :3:42:07 PM
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	35
25.00	Pumps	Solvent B Conc.	95
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	35
35.00	Pumps	Solvent B Conc.	35
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

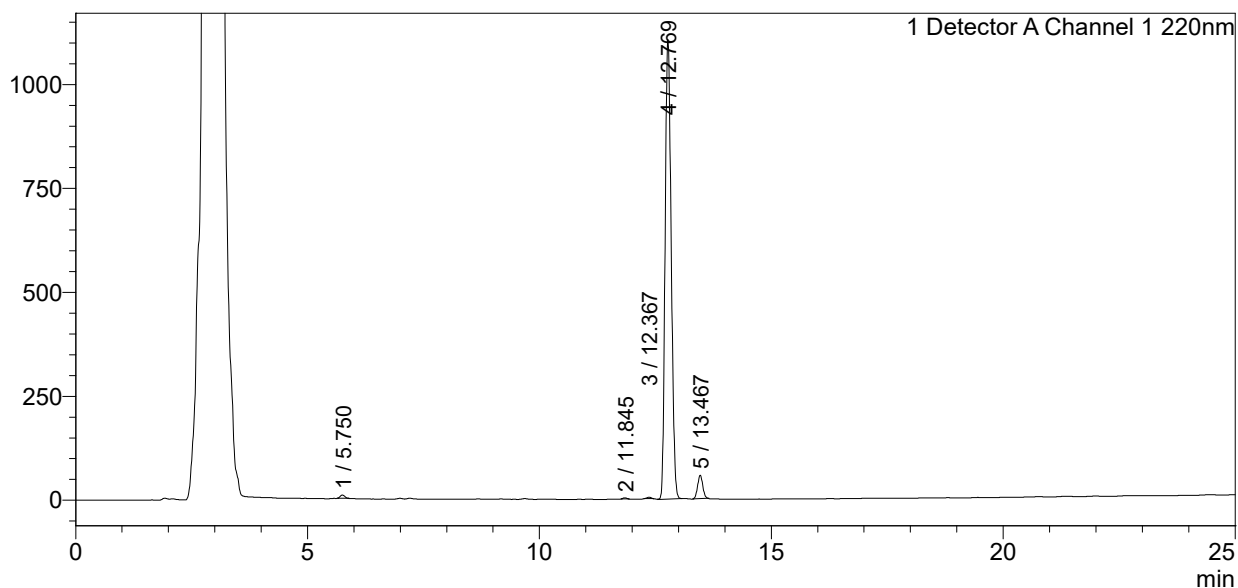

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.750	51170	7763	0.485
2	11.845	13609	2581	0.129
3	12.367	21473	3333	0.203
4	12.769	10036852	1106467	95.086
5	13.467	432490	56305	4.097
Total		10555594	1176450	100.000