


Mass Spectrum

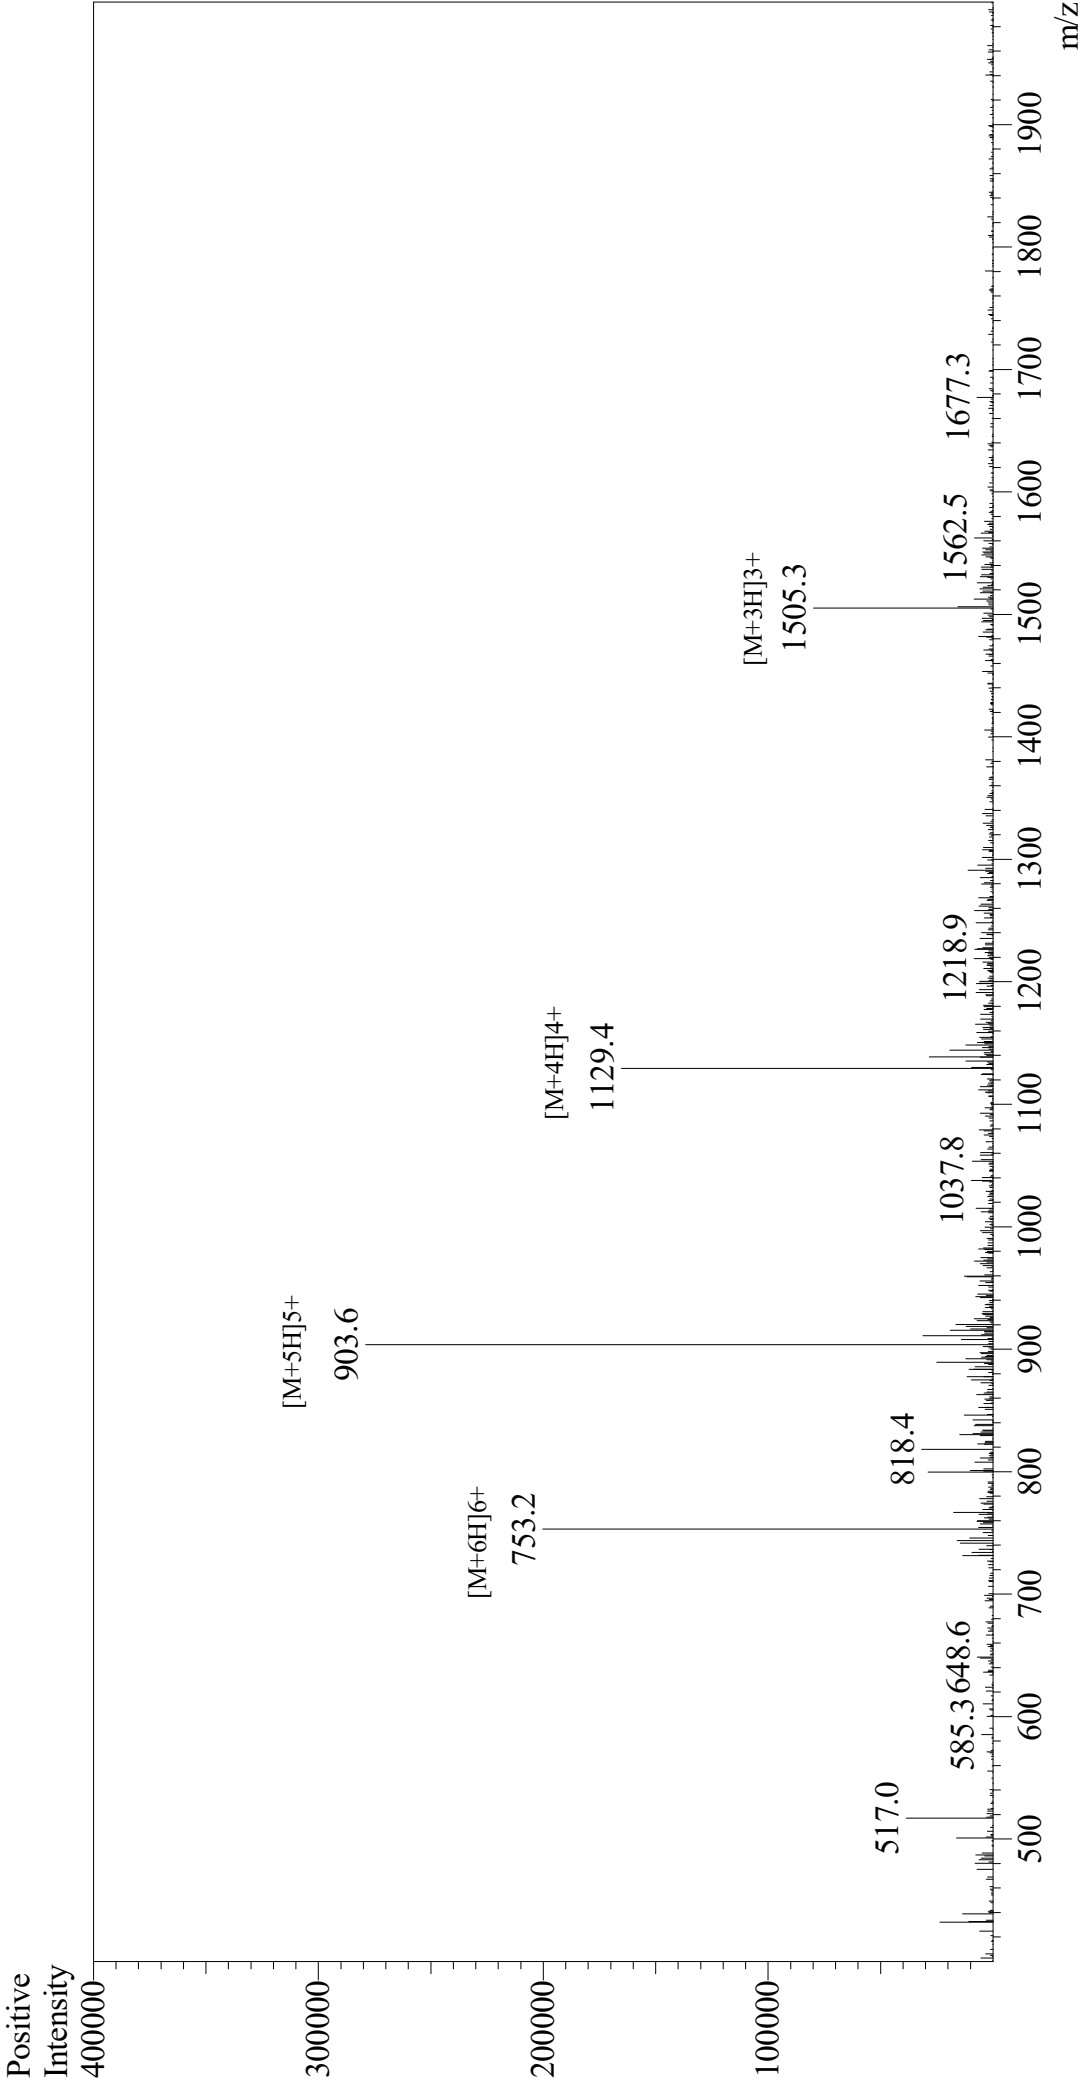

Sample Information	Equipment	: GK11010007
Month-Day Processed :	Interface Bias	: +4.5 kV
Time Processed :	Drying Gas Flow	: 5 L/min
Injection Volume :	T.Flow	: 0.2 ml/min
Sample Name :	B.conc	: 50% H2O/50% MeOH
Cat No. :	Interface	: ESI
Lot No. :	Nebulizing Gas Flow	: 1.5 L/min
Theoretical MW :	CDL Temp	: 250
Observed MW :	Block Temp	: 200

Month-Day Processed :	04/06/21
Time Processed :	22:15:09
Injection Volume :	0.4
Sample Name :	β-Amyloid (1-42), human
Cat No. :	RP10017
Lot No. :	E8091221C
Theoretical MW :	4514.10
Observed MW :	4513.0