

Sample Name:[Leu5]-Enkephalin
 Cat No :RP10884
 Lot No :E1973921E
 Time Processed :4:44:45 PM
 Month-Day-Year Processed :05/13/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

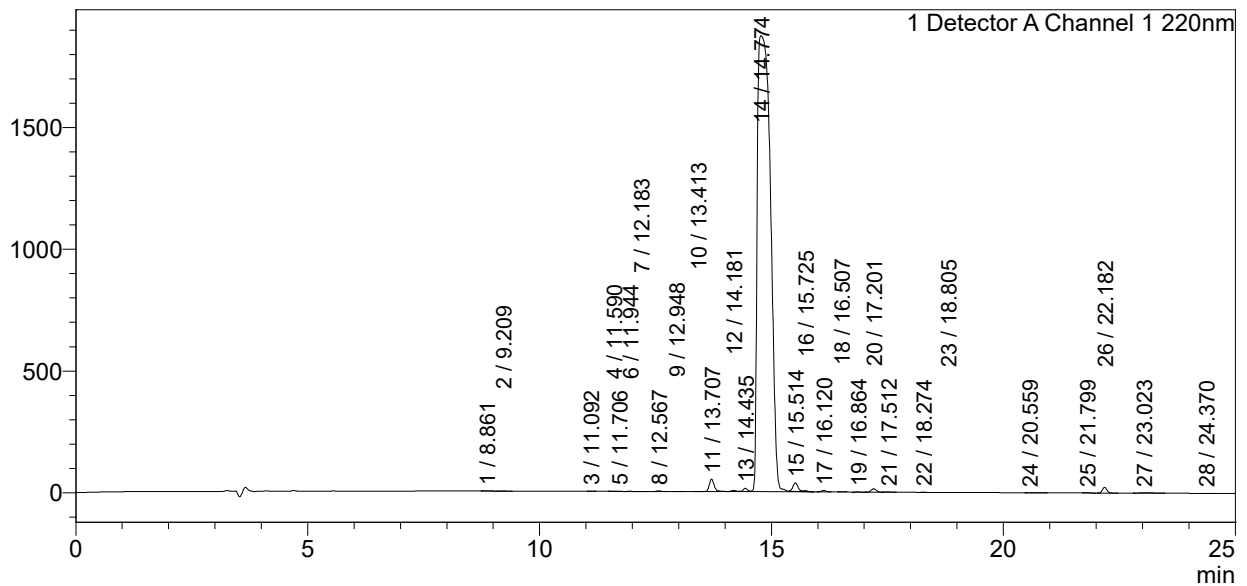

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.861	3868	493	0.010
2	9.209	2788	377	0.007
3	11.092	1691	308	0.004
4	11.590	1064	168	0.003
5	11.706	1325	212	0.003
6	11.944	1553	272	0.004
7	12.183	1282	212	0.003
8	12.567	16991	2663	0.045
9	12.948	1175	202	0.003
10	13.413	1248	203	0.003
11	13.707	391487	51404	1.032
12	14.181	42413	5133	0.112
13	14.435	94390	13715	0.249
14	14.774	36735360	1874761	96.868
15	15.514	257647	34601	0.679
16	15.725	25366	3997	0.067

Peak#	Ret. Time	Area	Height	Area%
17	16.120	38296	5702	0.101
18	16.507	1626	313	0.004
19	16.864	3750	474	0.010
20	17.201	101477	13981	0.268
21	17.512	7223	995	0.019
22	18.274	2810	307	0.007
23	18.805	1677	265	0.004
24	20.559	2835	179	0.007
25	21.799	1379	166	0.004
26	22.182	163217	23843	0.430
27	23.023	17907	797	0.047
28	24.370	1213	167	0.003
Total		37923058	2035910	100.000