

Sample Name : Colivelin  
 Cat. No. :RP20167  
 Lot. No. :E4838219I  
 Time Processed :12:59:38  
 Month-Day-Year Processed :09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

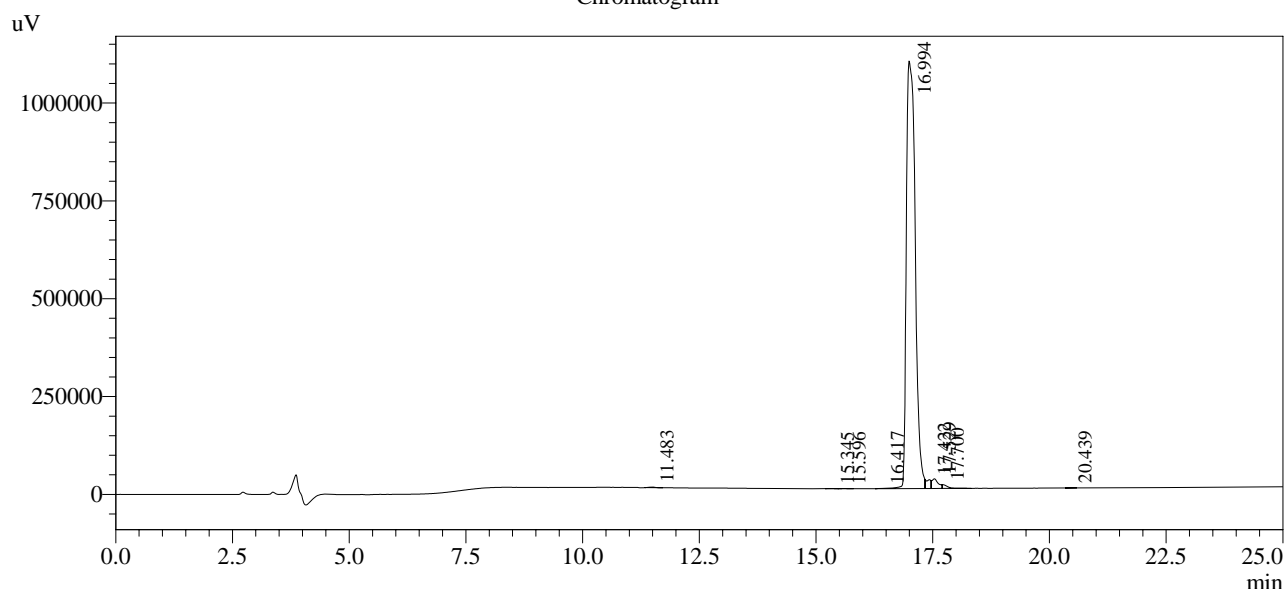

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.483	11238	1406	0.075
2	15.345	2814	456	0.019
3	15.596	2980	443	0.020
4	16.417	4284	558	0.029
5	16.994	14388358	1091877	96.645
6	17.422	166127	21990	1.116
7	17.529	234170	23798	1.573
8	17.700	74948	9599	0.503
9	20.439	2862	416	0.019
Total		14887780	1150544	100.000