

Sample Name: Bradykinin (1-7)  
 Cat. No. : RP11133  
 Lot. No. : E2563919J  
 Time Processed : 5:35:40  
 Month-Day-Year Processed : 10/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK12010012

<Chromatogram>

mV

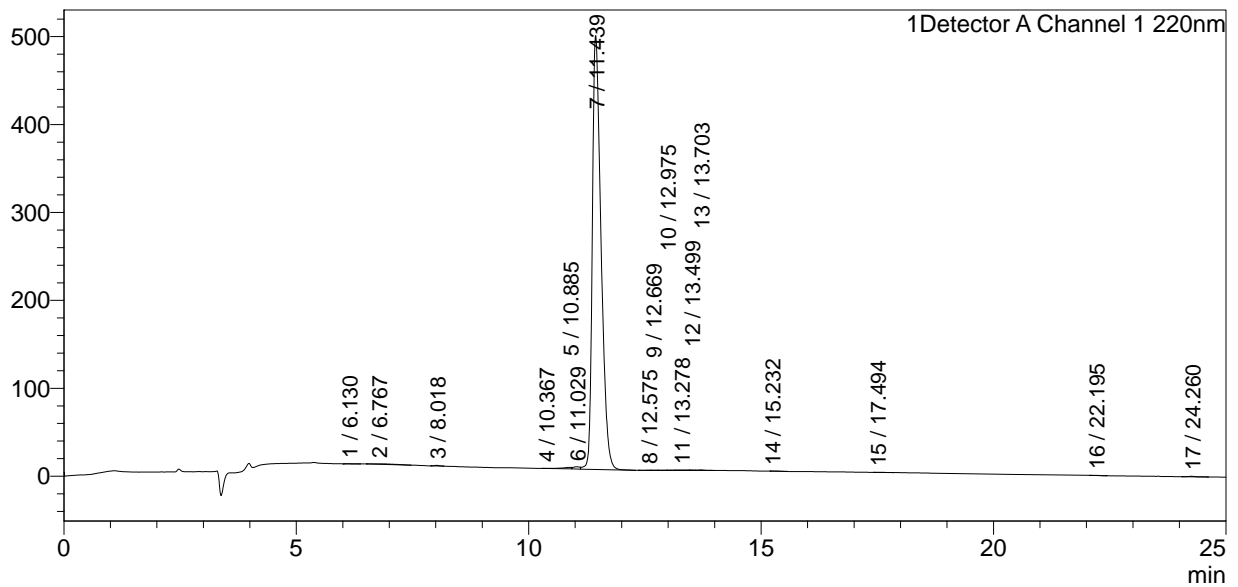

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.130	1143	148	0.018
2	6.767	19170	520	0.293
3	8.018	4536	746	0.069
4	10.367	1024	139	0.016
5	10.885	19959	1689	0.306
6	11.029	25567	2581	0.391
7	11.439	6417429	493449	98.234
8	12.575	2588	286	0.040
9	12.669	2319	298	0.035
10	12.975	4828	397	0.074
11	13.278	11489	558	0.176
12	13.499	3106	444	0.048
13	13.703	7043	602	0.108
14	15.232	1933	77	0.030
15	17.494	1760	127	0.027

Peak#	Ret. Time	Area	Height	Area%
16	22.195	2514	327	0.038
17	24.260	6380	619	0.098
Total		6532788	503006	100.000