

Sample Name :Neurotensin (8-13)
Cat No. :RP10442
Lot No. :E4808319I
Time Processed :2:40:44
Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
Equipment:ZJ17010507

<Chromatogram>

mV

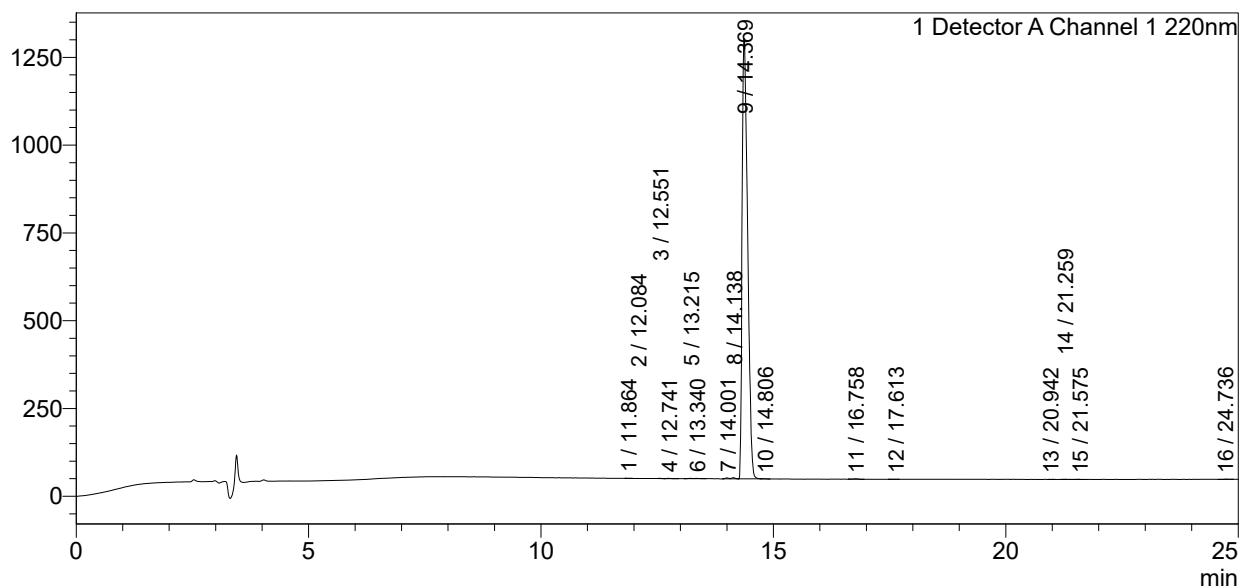

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.864	1738	284	0.017
2	12.084	3284	233	0.032
3	12.551	4387	833	0.042
4	12.741	5460	891	0.053
5	13.215	5385	891	0.052
6	13.340	5670	784	0.055
7	14.001	12820	2543	0.124
8	14.138	16804	3199	0.163
9	14.369	10241908	1253974	99.215
10	14.806	2688	589	0.026
11	16.758	8681	1273	0.084
12	17.613	2013	349	0.019
13	20.942	1132	207	0.011
14	21.259	3104	314	0.030
15	21.575	2997	297	0.029

Peak#	Ret. Time	Area	Height	Area%
16	24.736	4910	519	0.048
Total		10322983	1267181	100.000