

Sample Name :Melittin
 Cat. No. : RP10290
 Lot. No. : E6048520K
 Time Processed :8:59:23 AM
 Month-Day-Year Processed :11/12/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

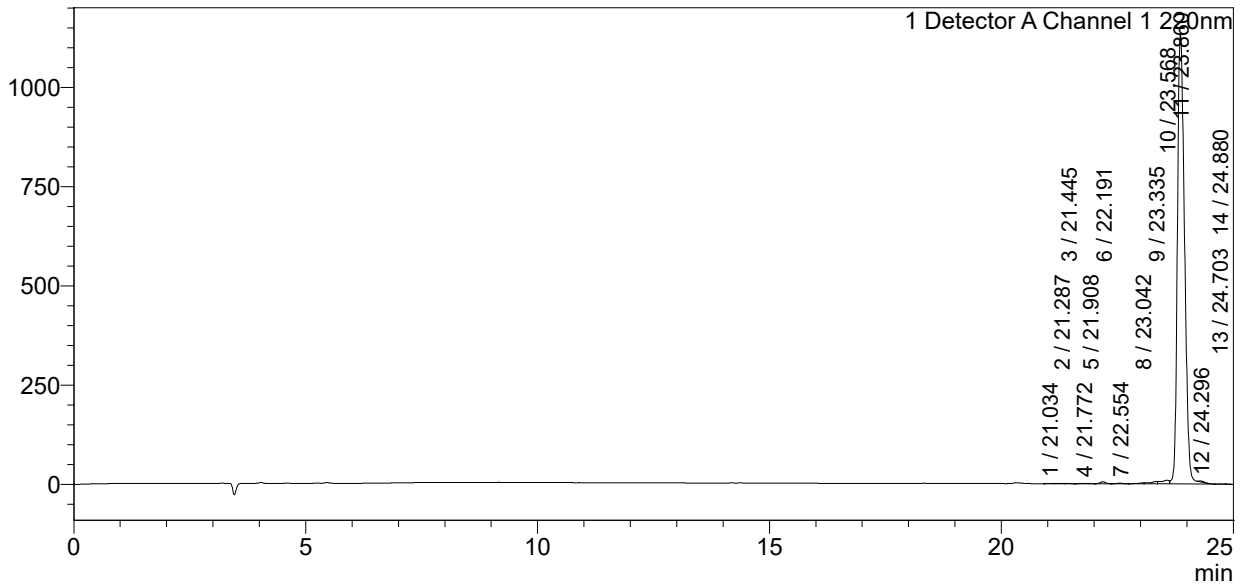

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	21.034	5454	633	0.044
2	21.287	4521	379	0.037
3	21.445	4767	648	0.039
4	21.772	9938	1028	0.080
5	21.908	3928	712	0.032
6	22.191	42084	5068	0.340
7	22.554	14368	1580	0.116
8	23.042	23070	2313	0.186
9	23.335	65840	5651	0.532
10	23.568	116740	9198	0.943
11	23.860	12067143	1134334	97.473
12	24.296	18350	2442	0.148
13	24.703	2189	320	0.018
14	24.880	1646	293	0.013
Total		12380039	1164597	100.000