


Sample Name :SV40 large T antigen NLS  
 Cat No. : RP20414  
 Lot No. : PE9271703  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

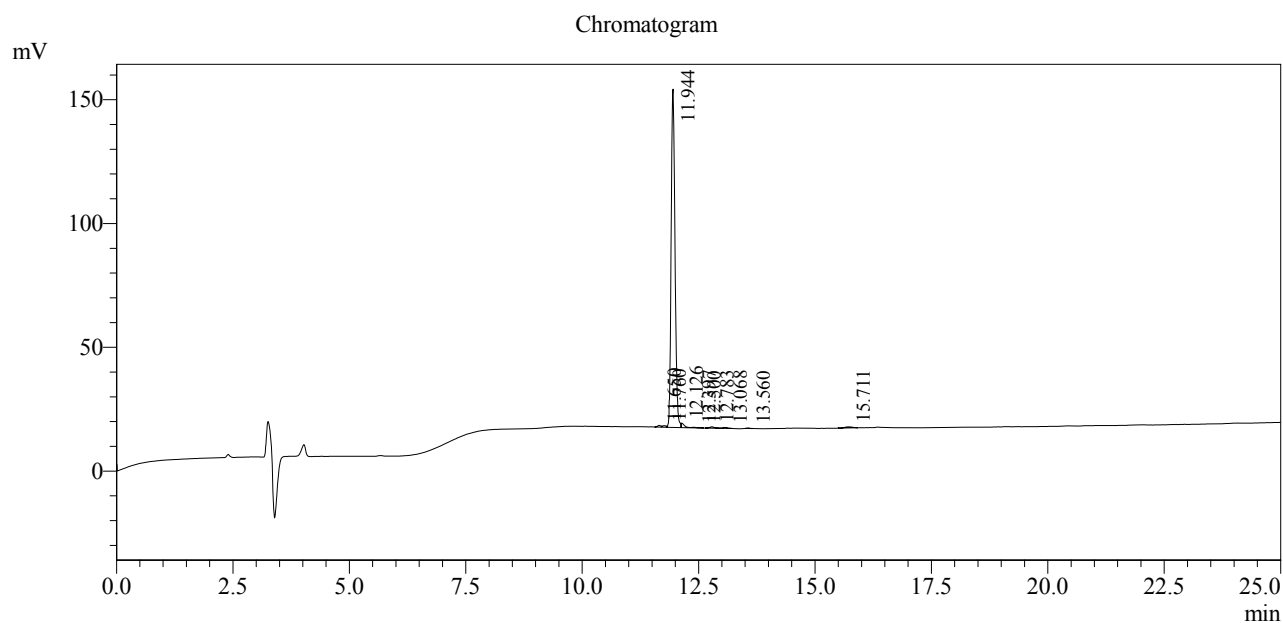

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.650	3660	678	0.449
2	11.760	3512	615	0.431
3	11.944	786221	136622	96.403
4	12.126	7665	1787	0.940
5	12.397	1736	224	0.213
6	12.500	186	45	0.023
7	12.783	4224	547	0.518
8	13.068	2463	360	0.302
9	13.560	885	195	0.109
10	15.711	5002	448	0.613
Total		815553	141521	100.000