

Sample Name :[Des-Arg<sup>9</sup>]-Bradykinin  
 Cat No. :RP13625  
 Lot No. :E5168719G  
 Time Processed :8:45:21  
 Month-Day-Year Processed :07/18/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

### <Chromatogram>

mV

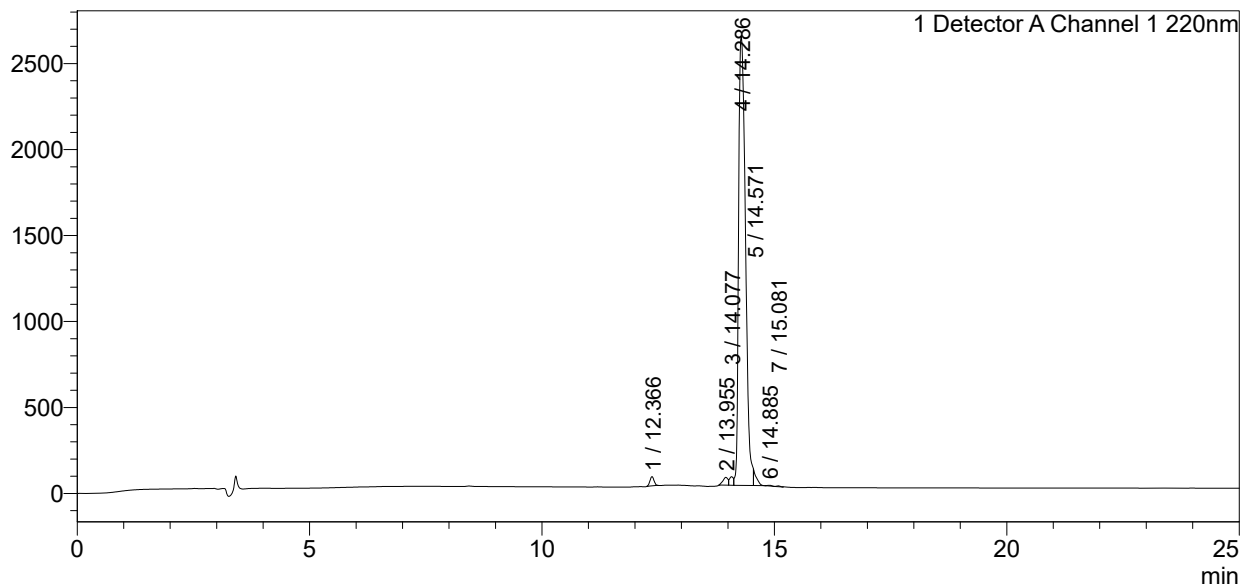

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.366	325405	53929	1.154
2	13.955	352718	45980	1.251
3	14.077	282911	49970	1.004
4	14.286	26798169	2611030	95.072
5	14.571	379350	78947	1.346
6	14.885	24275	4008	0.086
7	15.081	24408	4952	0.087
Total		28187234	2848816	100.000