

Sample Name : β -Amyloid (1-28)
 Cat. No. : RP10002
 Lot. No. : PE1861810
 Time Processed : 15:40:03
 Month-Day-Year Processed : 10/12/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

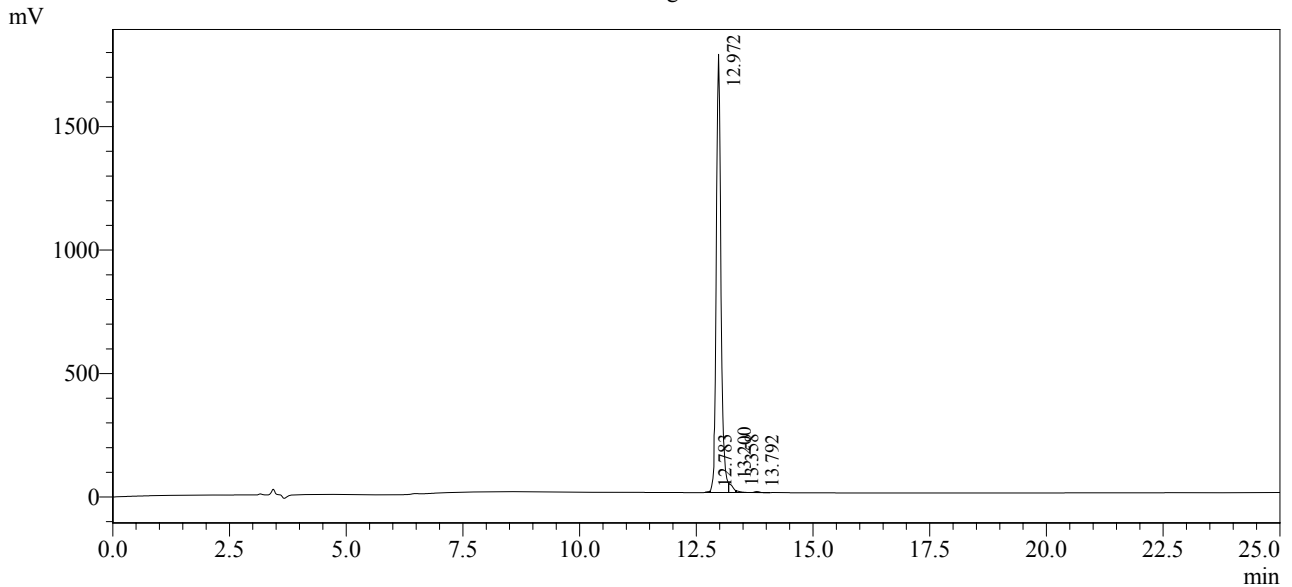

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.783	14460	3984	0.113
2	12.972	12448234	1774772	97.682
3	13.200	213373	35637	1.674
4	13.358	39204	6882	0.308
5	13.792	28391	3874	0.223
Total		12743663	1825149	100.000