

Sample Name : Neuromedin B
 Cat No.: RP10507
 Lot No.: E2737820K
 Time Processed : 21:23:41
 Month-Day-Year Processed : 11/29/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

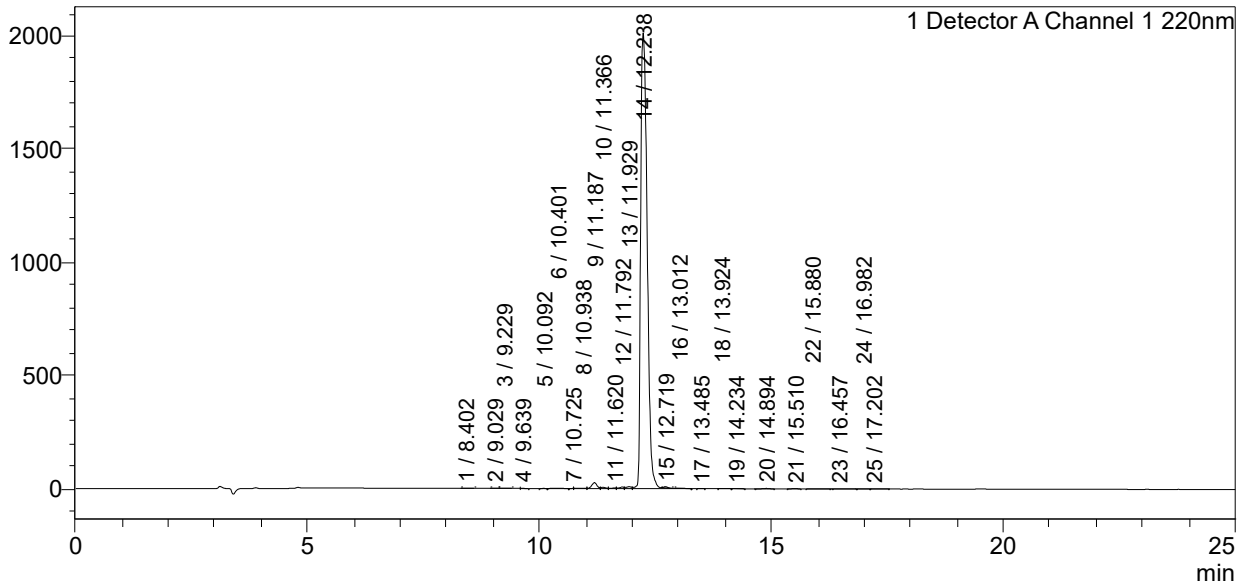

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.402	1036	124	0.005
2	9.029	1372	178	0.007
3	9.229	1097	144	0.005
4	9.639	1006	202	0.005
5	10.092	1670	233	0.008
6	10.401	10041	1007	0.050
7	10.725	1587	288	0.008
8	10.938	9589	818	0.048
9	11.187	201583	25988	1.007
10	11.366	38706	5361	0.193
11	11.620	17082	1988	0.085
12	11.792	44936	6415	0.224
13	11.929	66572	7736	0.332
14	12.238	19550468	2012960	97.621
15	12.719	32813	5673	0.164

Peak#	Ret. Time	Area	Height	Area%
16	13.012	2737	187	0.014
17	13.485	1787	360	0.009
18	13.924	2209	308	0.011
19	14.234	4351	521	0.022
20	14.894	11815	1665	0.059
21	15.510	7659	1197	0.038
22	15.880	3471	243	0.017
23	16.457	4368	314	0.022
24	16.982	5249	411	0.026
25	17.202	3672	237	0.018
Total		20026877	2074558	100.000