

Sample Name : Mas7
 Cat No. : RP10602
 Lot No. : E5881320K
 Time Processed :1:56:23 AM
 Month-Day-Year Processed :11/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010140

<Chromatogram>

mV

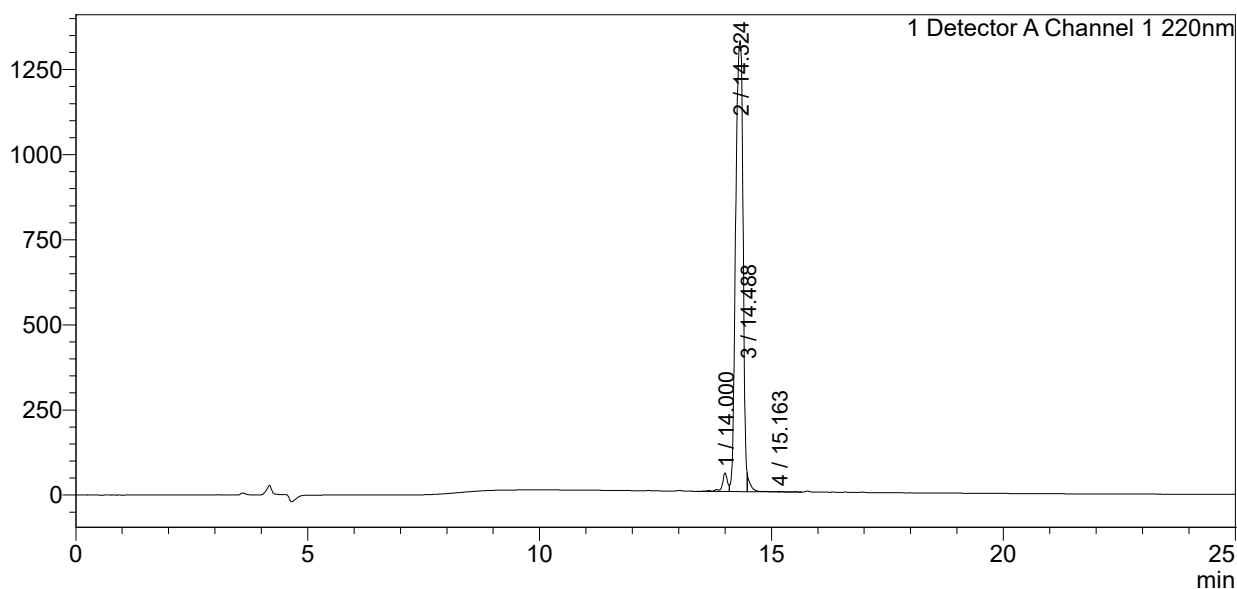

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.000	431177	55132	2.843
2	14.324	14504318	1325073	95.633
3	14.488	227385	47508	1.499
4	15.163	3713	258	0.024
Total		15166593	1427971	100.000