

Sample Name :Peptide YY (PYY), human
Cat No. :RP10355
Lot No. :PE0261901

Time Processed : 2:16:53
Month-Day-Year Processed : 01/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

<Chromatogram>

mV

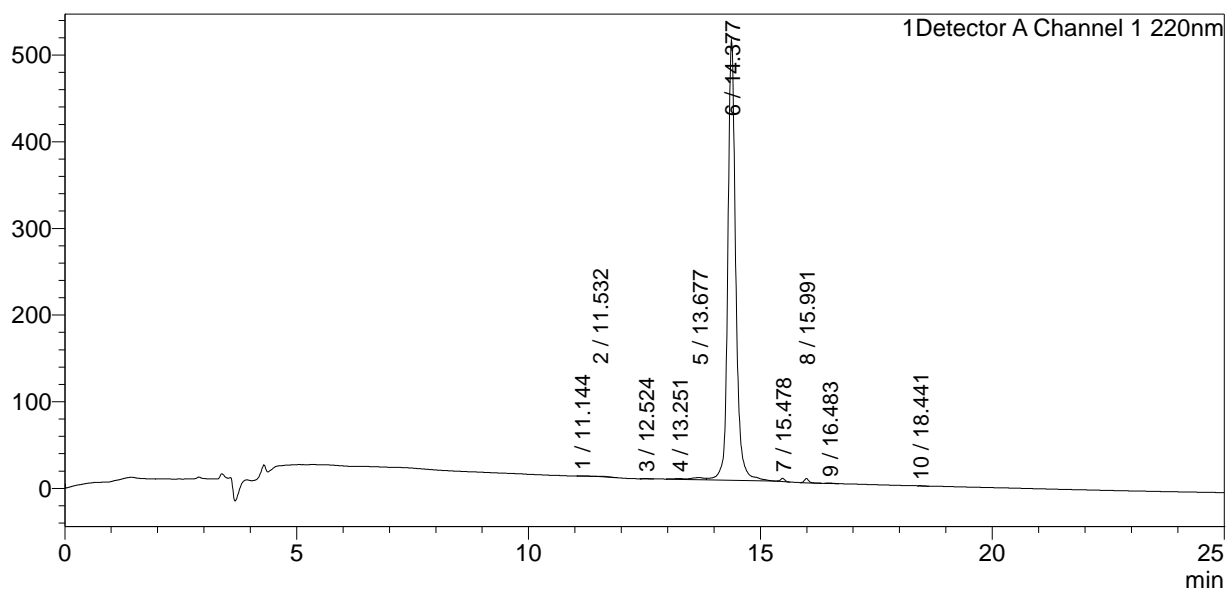

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.144	2329	205	0.038
2	11.532	9733	473	0.158
3	12.524	4246	552	0.069
4	13.251	12068	812	0.196
5	13.677	46909	2396	0.761
6	14.377	6026960	508209	97.834
7	15.478	22461	3756	0.365
8	15.991	31230	4821	0.507
9	16.483	3430	417	0.056
10	18.441	1027	128	0.017
Total		6160394	521771	100.000