

Sample Name : Dynorphin A(1-13),porcine
 Cat. No. : RP20492
 Lot. No. : PE4281811
 Time Processed :22:54:55
 Month-Day-Year Processed :11/06/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

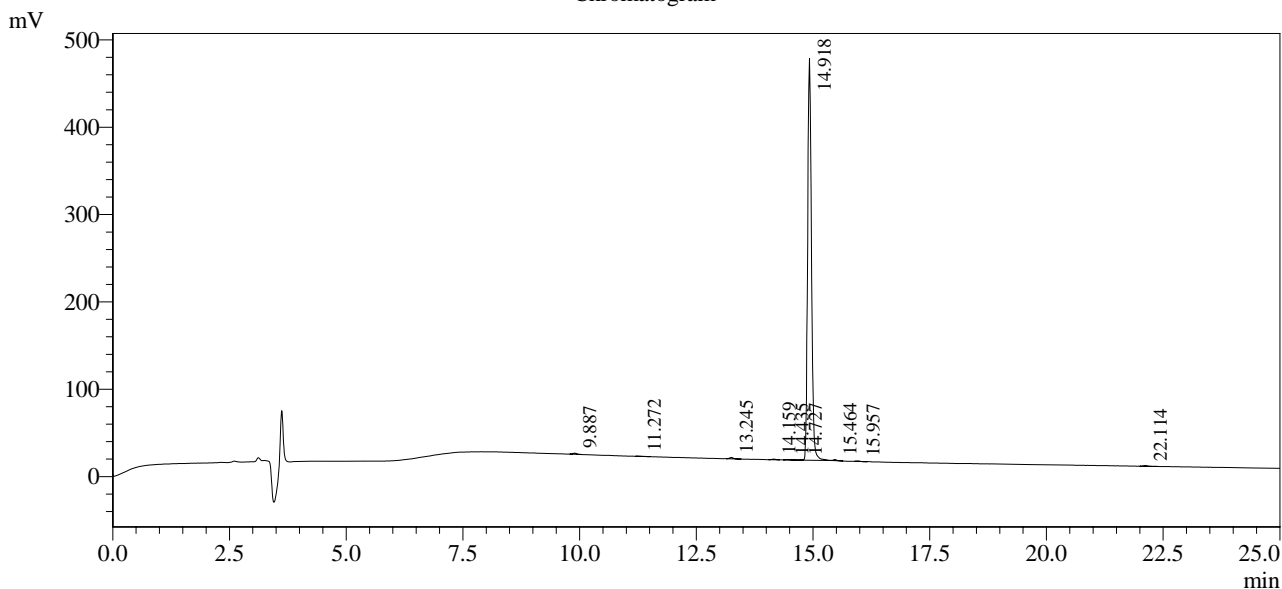

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.887	7121	1335	0.266
2	11.272	3316	479	0.124
3	13.245	9361	1597	0.350
4	14.159	4063	762	0.152
5	14.435	1902	298	0.071
6	14.727	1429	242	0.053
7	14.918	2633289	460253	98.437
8	15.464	6175	1256	0.231
9	15.957	3268	635	0.122
10	22.114	5187	718	0.194
Total		2675111	467575	100.000