

Sample Name :Beta-Amyloid(1-14),mouse,rat
Cat No.: RP20505
Lot No.: E4974019I
Time Processed:10:44:24
Month-Day-Year Processed:09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
Equipment:ZJ19010014

<Chromatogram>

mV

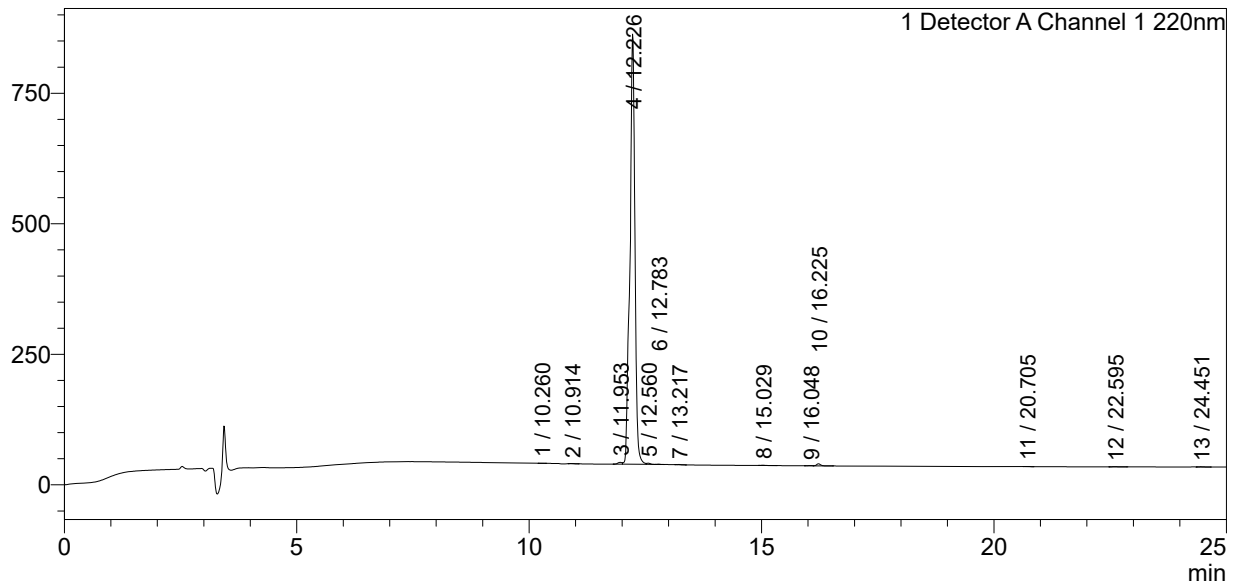

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.260	1371	306	0.022
2	10.914	2588	547	0.041
3	11.953	22880	3614	0.365
4	12.226	6186210	823814	98.677
5	12.560	12163	2237	0.194
6	12.783	2421	506	0.039
7	13.217	2277	443	0.036
8	15.029	3915	600	0.062
9	16.048	3339	557	0.053
10	16.225	24506	4059	0.391
11	20.705	2135	360	0.034
12	22.595	2896	413	0.046
13	24.451	2437	357	0.039
Total		6269138	837813	100.000