

Sample Name :Chemerin-9 (149-157)
 Cat No. :RP20248
 Lot No. :E5710819F
 Time Processed :14:04:47
 Month-Day-Year Processed :07/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

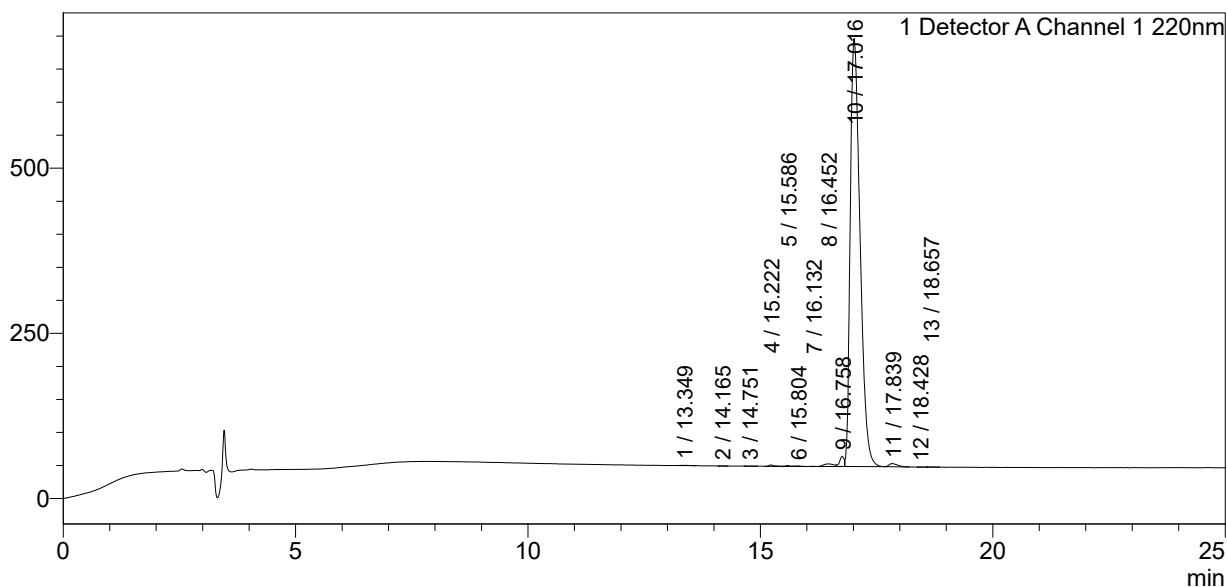

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.349	4920	324	0.050
2	14.165	2058	379	0.021
3	14.751	4114	568	0.042
4	15.222	20451	2242	0.209
5	15.586	10263	1341	0.105
6	15.804	7227	734	0.074
7	16.132	2352	430	0.024
8	16.452	62960	4017	0.643
9	16.758	103242	15411	1.054
10	17.016	9512446	647991	97.120
11	17.839	59894	4760	0.612
12	18.428	1551	241	0.016
13	18.657	2999	384	0.031
Total		9794479	678823	100.000