

Sample Name :Magainin 2
 Cat No : RP11232
 Lot No : E8973120J
 Time Processed :1:24:09 AM
 Month-Day-Year Processed :11/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
41.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

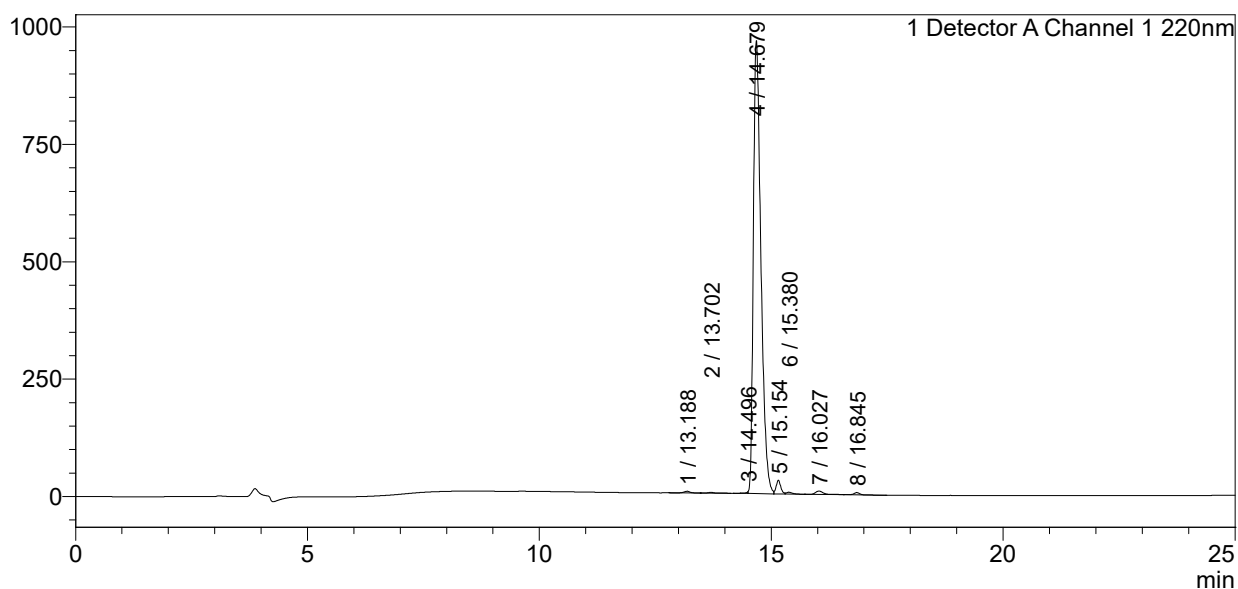

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.188	33593	3671	0.297
2	13.702	17592	1658	0.155
3	14.496	13837	2839	0.122
4	14.679	10902320	964752	96.235
5	15.154	199014	28840	1.757
6	15.380	32932	3864	0.291
7	16.027	87599	7160	0.773
8	16.845	41908	4989	0.370
Total		11328794	1017773	100.000