

Sample Name :BNP(1-45), mouse  
Cat No.: RP20365  
Lot No.: E6203020A  
Time Processed :3:03:54  
Month-Day-Year Processed :02/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
Equipment:ZJ19010014

### <Chromatogram>

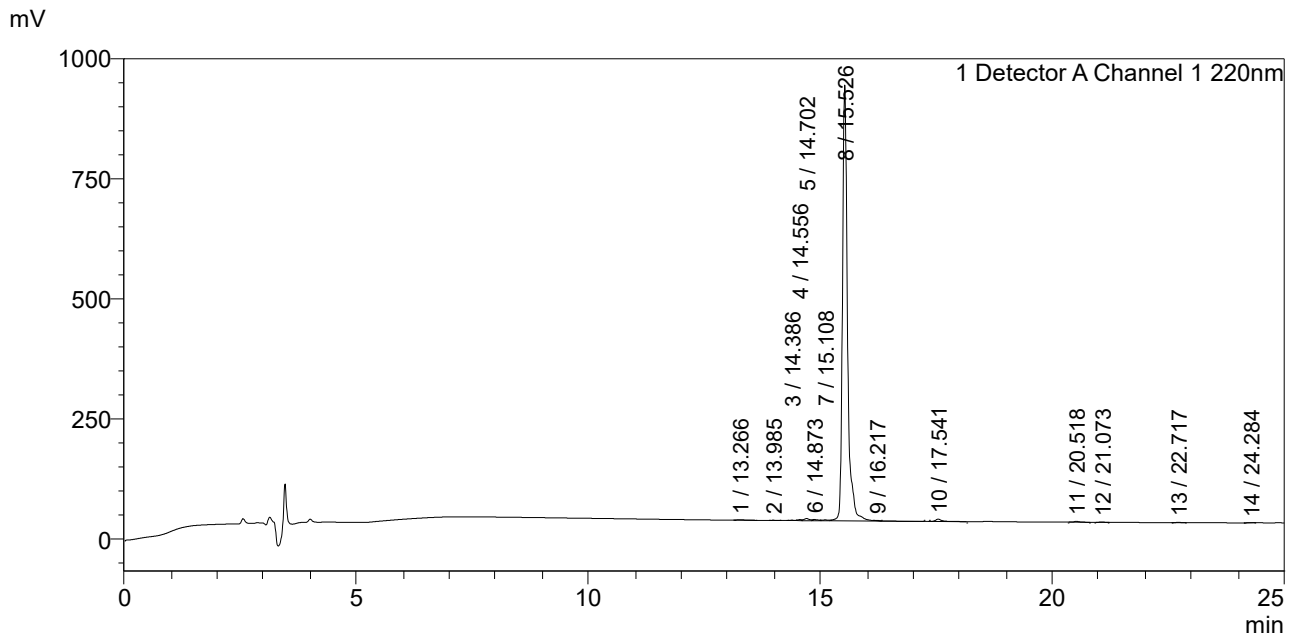

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.266	8687	890	0.122
2	13.985	2026	376	0.029
3	14.386	4065	717	0.057
4	14.556	13842	2045	0.195
5	14.702	35195	4313	0.496
6	14.873	23498	2351	0.331
7	15.108	17543	1791	0.247
8	15.526	6922890	906530	97.469
9	16.217	2093	461	0.029
10	17.541	47446	4929	0.668
11	20.518	14349	1816	0.202
12	21.073	4032	620	0.057
13	22.717	3887	472	0.055
14	24.284	3105	498	0.044
Total		7102659	927808	100.000