

Sample Name :Bradykinin
 Cat No. :RP11129
 Lot No. :E2688221A
 Time Processed :9:48:11 AM
 Month-Day-Year Processed :01/06/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

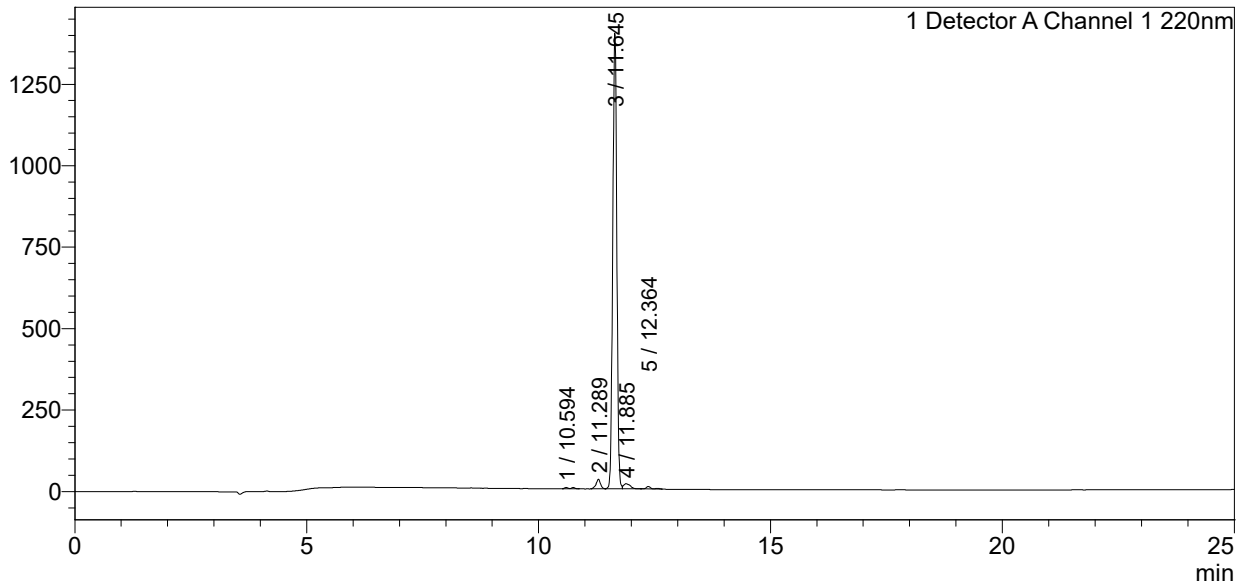

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.594	34411	3790	0.383
2	11.289	196544	29286	2.186
3	11.645	8544193	1399041	95.036
4	11.885	158806	15852	1.766
5	12.364	56547	7638	0.629
Total		8990500	1455608	100.000