


Mass Spectrum

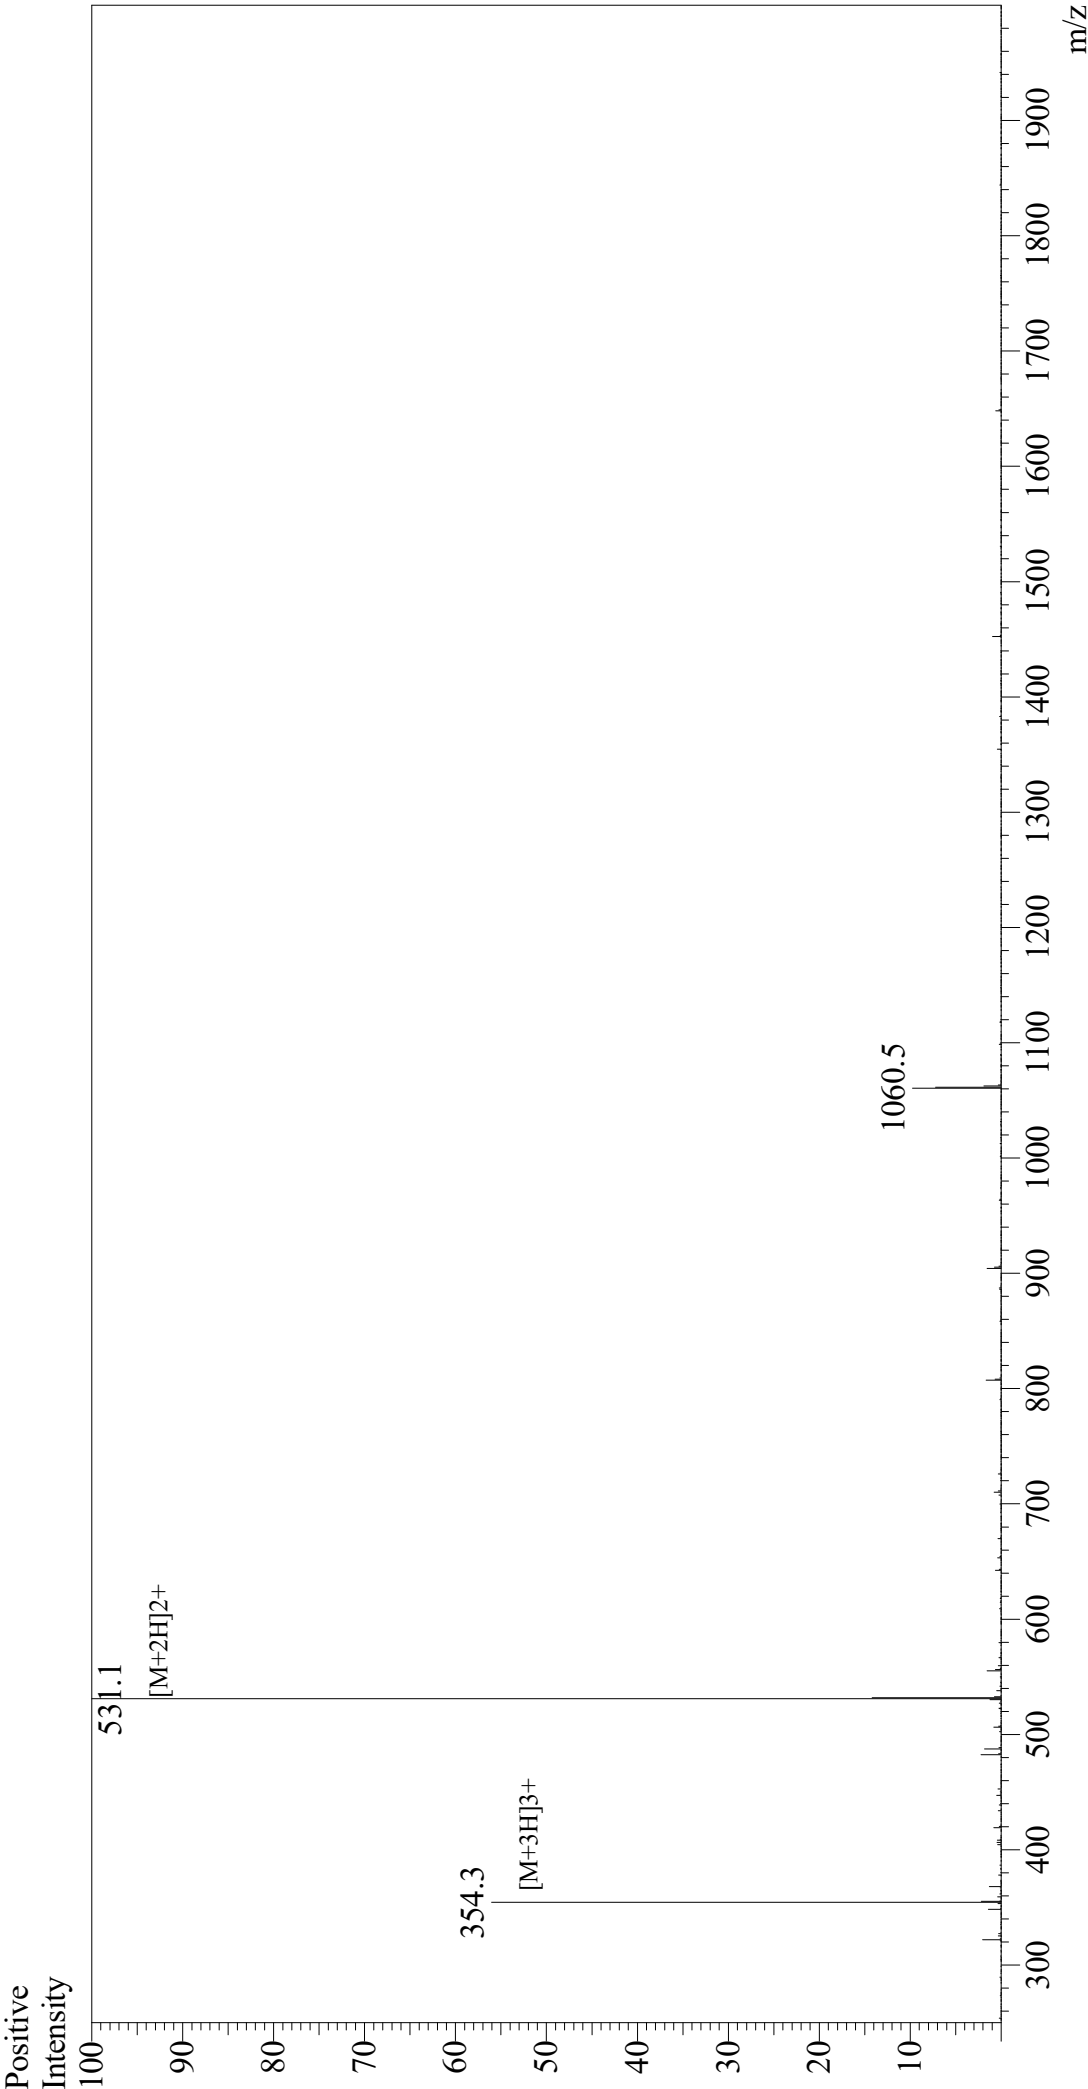

Sample Information		Interface		Equipment	
Month-Day Processed :	01/05/21	Nebulizing Gas Flow : 1.5L/min		: GK11010007	
Time Processed :	9:31:37 AM	CDL Temp : 250		Interface Bias : +3.5 kV	
Injection Volume :	0.3	Block Temp : 200		Drying Gas Flow : 5 L/min	
Sample Name :	Bradykinin			T.Flow : 0.2 ml/min	
Cat No. :	RP111129			B.conc : 50%H2O/50%MeOH	
Lot No. :	E2688221A				
Theoretical MW :	1060.20				
Observed MW :	1060.2				