

Sample Name :OVA Peptide (257-264)
 Cat No. :RP10611
 Lot No. :E4630221H
 Time Processed :5:41:32
 Month-Day-Year Processed :08/10/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

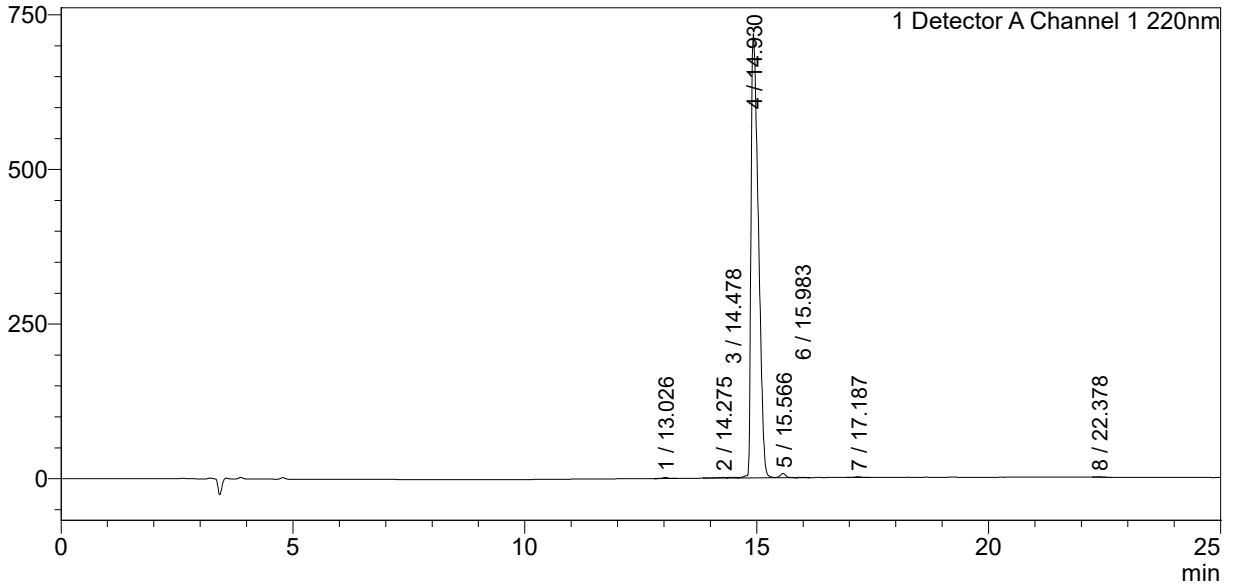

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.026	12322	1600	0.153
2	14.275	13494	995	0.167
3	14.478	13916	1232	0.172
4	14.930	7949994	705182	98.535
5	15.566	60002	6654	0.744
6	15.983	4828	606	0.060
7	17.187	8904	1029	0.110
8	22.378	4709	699	0.058
Total		8068168	717997	100.000