

Sample Name : Melittin
 Cat. No. : RP10290
 Lot. No. : E5697319F
 Time Processed : 6:54:48
 Month-Day-Year Processed : 06/29/2019
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

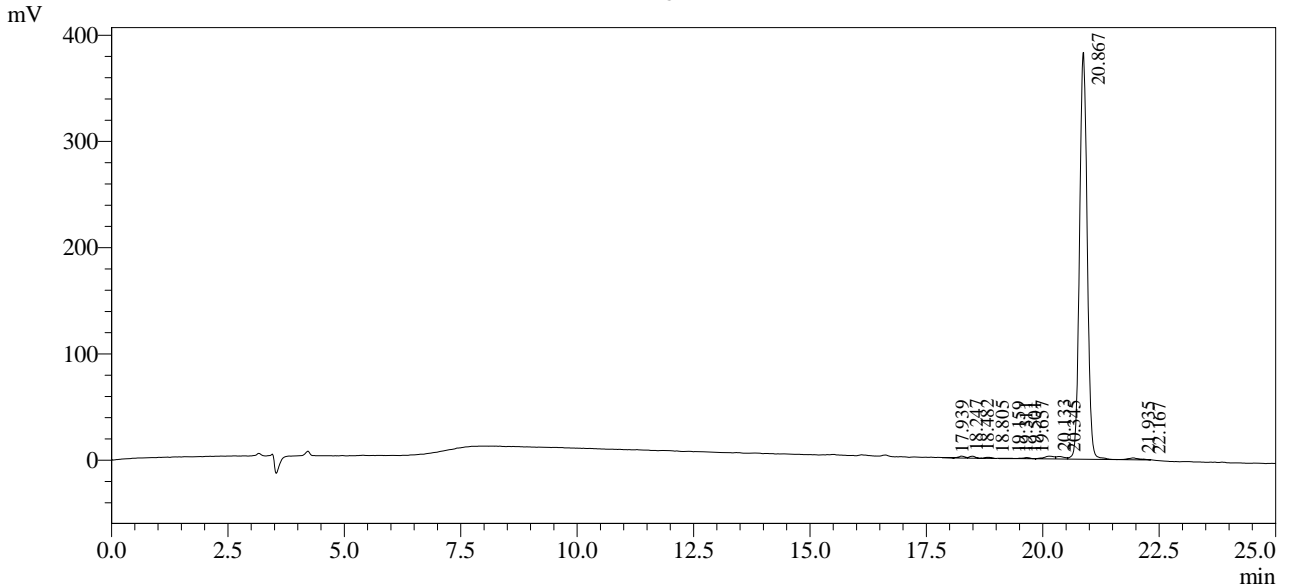

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.939	2251	303	0.049
2	18.247	17930	1833	0.394
3	18.482	16298	1860	0.358
4	18.805	10756	1081	0.236
5	19.159	2928	309	0.064
6	19.311	2678	358	0.059
7	19.501	1963	429	0.043
8	19.657	9821	1055	0.216
9	20.133	38588	2522	0.848
10	20.345	28847	2369	0.634
11	20.867	4389359	382860	96.415
12	21.935	27587	1759	0.606
13	22.167	3542	651	0.078
Total		4552548	397388	100.000