

Sample Name :Adrenocorticotrophic Hormone (ACTH) (4-10), human  
 Cat No. :RP11308  
 Lot No. :E4725119I  
 Time Processed :10:58:24 AM  
 Month-Day-Year Processed :09/22/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
30.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

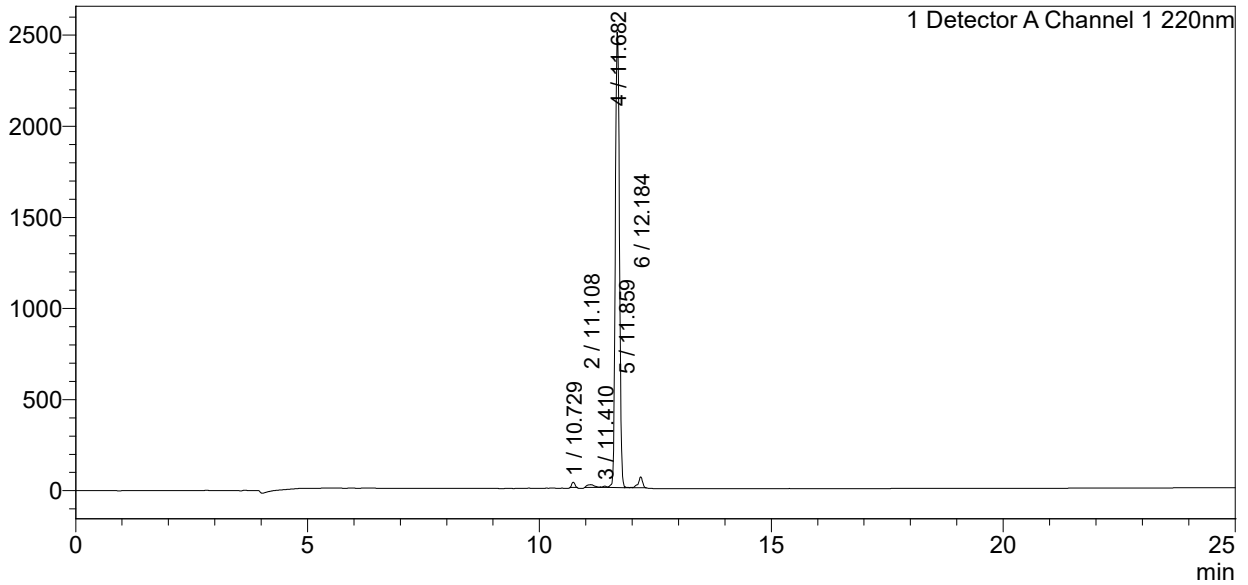

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.729	131865	29055	0.818
2	11.108	179840	15456	1.116
3	11.410	46861	8031	0.291
4	11.682	15382544	2499983	95.461
5	11.859	7044	2136	0.044
6	12.184	365850	59503	2.270
Total		16114004	2614164	100.000