

Sample Name :Arg-Gly-Asp-Cys
 Cat. No. : RP10860
 Lot. No. :E0172520A
 Time Processed :14:28:50
 Month-Day-Year Processed :01/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	0	
5.00	Pumps	Pump B Conc.	0	
20.00	Pumps	Pump B Conc.	30	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	0	
40.00	Pumps	Pump B Conc.	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

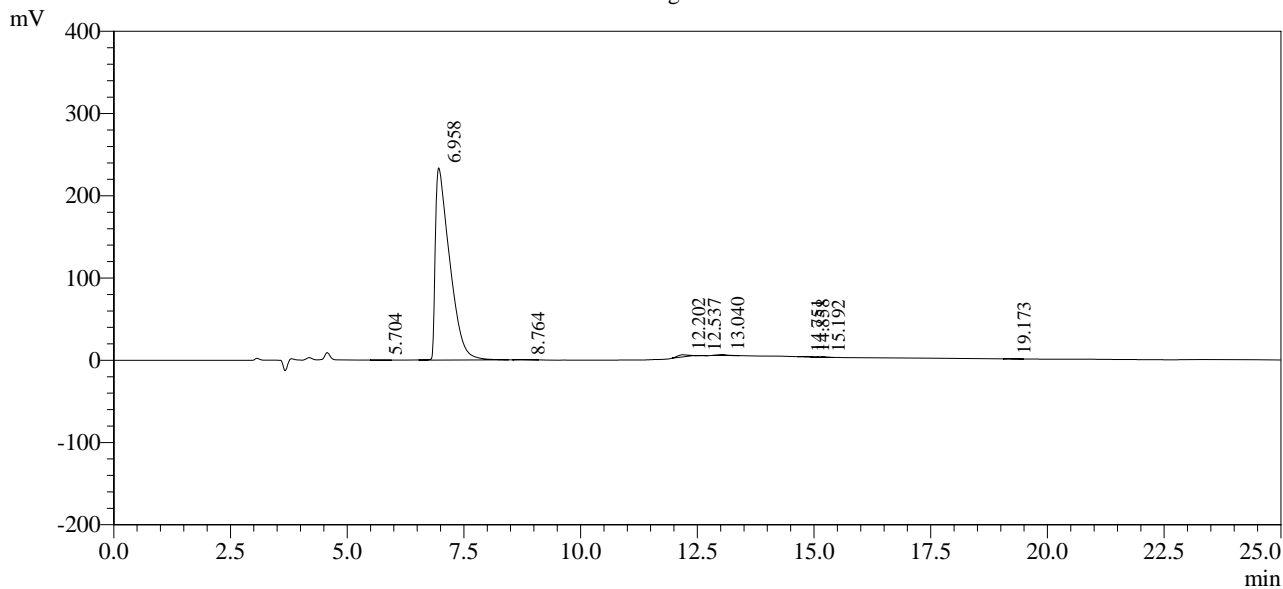

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.704	2719	288	0.053
2	6.958	5008580	233594	98.365
3	8.764	9418	677	0.185
4	12.202	40625	2625	0.798
5	12.537	2868	330	0.056
6	13.040	16562	1287	0.325
7	14.751	2632	390	0.052
8	14.858	2940	524	0.058
9	15.192	4188	593	0.082
10	19.173	1317	182	0.026
Total		5091850	240490	100.000