


# Mass Spectrum

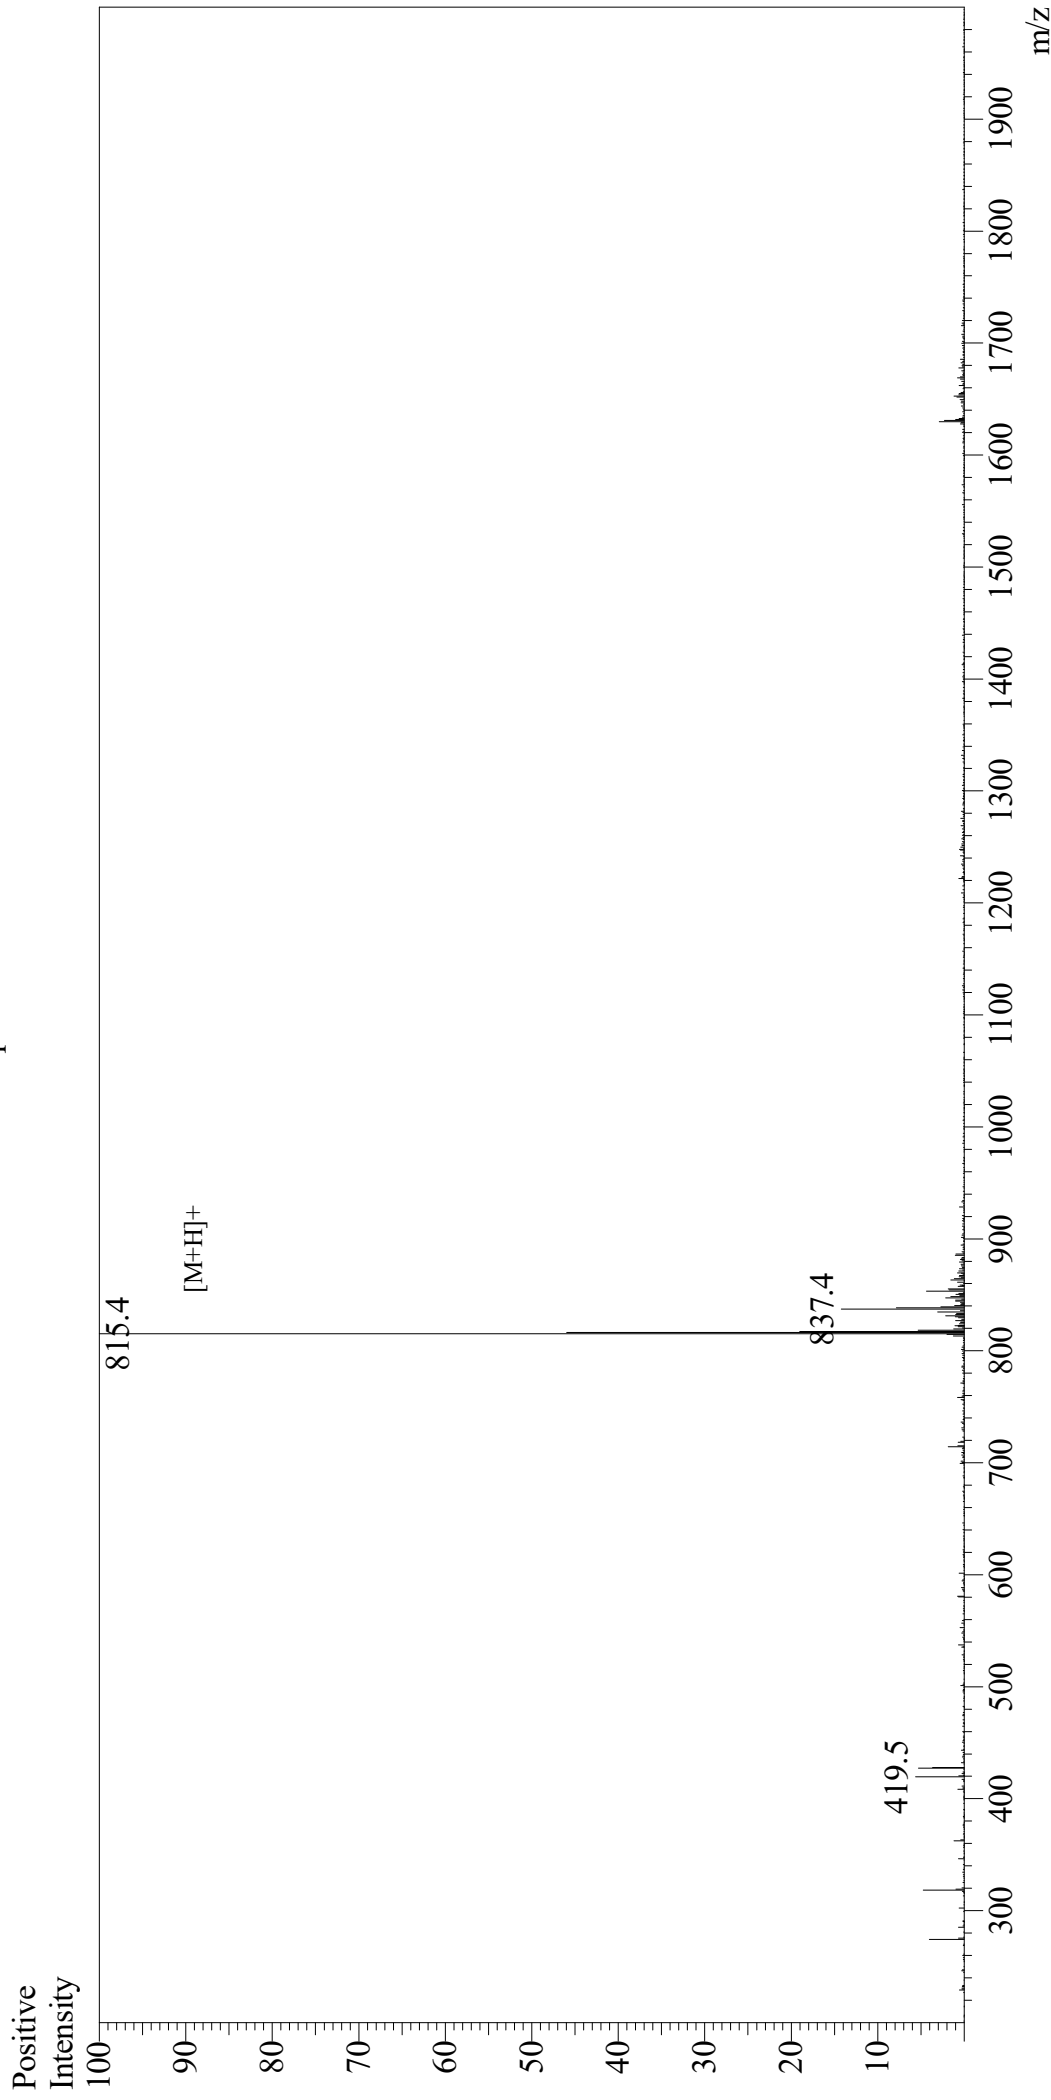

## Sample Information

User : Gary  
Month-Day Processed : 10/02/19  
Time Processed : 05:55:10 PM  
Injection Volume : 0.3  
Sample Name : HPV16 E7(86-93)  
Cat No. : RP20499  
Lot No. : E7085619J  
Theoretical MW : 815.10  
Observed MW : 814.4

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH